

# Human IL-3 ELISA Kit

Catalog Number KHC0031 (96 tests)

Pub. No. MAN0004084 Rev. 1.0

**CAUTION!** This kit contains materials with small quantities of sodium azide. Sodium azide reacts with lead and copper plumbing to form explosive metal azides. Upon disposal, flush drains with a large volume of water to prevent azide accumulation. Avoid ingestion and contact with eyes, skin and mucous membranes. In case of contact, rinse affected area with plenty of water. Observe all federal, state, and local regulations for disposal.

**Note:** For safety and biohazard guidelines, see the “Safety” appendix in the *ELISA Technical Guide* (Pub. no. MAN0006706). Read the Safety Data Sheets (SDSs) and follow the handling instructions. Wear appropriate protective eyewear, clothing, and gloves.

## Product description

The Invitrogen™ Human IL-3 ELISA Kit is a solid-phase sandwich Enzyme-Linked Immunosorbent Assay (ELISA). This assay is designed to detect and quantify the level of human IL-3 in human serum, plasma, buffered solution, or cell culture medium. The assay recognizes both natural and recombinant human IL-3.

Human IL-3 (Multi-CSF) is a 15-17 kDa glycosylated protein produced by activated T-lymphocytes and NK-cells. IL-3 stimulates the growth and differentiation of pluripotential hemopoietic stem cells that are progenitors of neutrophils, macrophages, megakaryocytes, erythrocytes, eosinophils, basophils, and mast cells.

## Contents and storage

Upon receipt, store the kit at 2°C to 8°C.

Contents	Cat. No. KHC0031 (96 tests)
Hu IL-3 Standard; lyophilized. Refer to vial label for quantity and reconstitution volume	2 vials
Standard Diluent Buffer; contains 15 mM sodium azide	25 mL
Hu IL-3 Antibody-Coated Wells, 96-well strip-well plate	1 plate
Hu IL-3 Biotin Conjugate; contains 15 mM sodium azide	11 mL
Streptavidin-Peroxidase (HRP), (100X); contains 3.3 mM thymol	0.125 mL
Streptavidin-Peroxidase (HRP) Diluent; contains 3.3 mM thymol	25 mL
Wash Buffer Concentrate (25X)	100 mL
Stabilized Chromogen, Tetramethylbenzidine (TMB)	25 mL
Stop Solution	25 mL
Plate Covers, adhesive strips	3

## Materials required but not supplied

- Distilled or deionized water
- Microtiter plate reader with software capable of measurement at or near 450 nm
- Plate washer—automated or manual (squirt bottle, manifold dispenser, or equivalent)
- Calibrated adjustable precision pipettes and glass or plastic tubes for diluting solutions

## Before you begin

**IMPORTANT!** Reagents are lot-specific. Do not mix or interchange different reagent lots from various kit lots.

- Review the **Procedural guidelines** and **Plate washing directions** in the *ELISA Technical Guide* available at [thermofisher.com](http://thermofisher.com).
- Allow reagents to reach room temperature before use. Mix to redissolve any precipitated salts.

## Prepare 1X Wash Buffer

1. Dilute 16 mL of Wash Buffer Concentrate (25X) with 384 mL of deionized or distilled water. Label as 1X Wash Buffer.
2. Store the concentrate and 1X Wash Buffer in the refrigerator. Use the diluted buffer within 14 days.

## Sample preparation guidelines

- Refer to the *ELISA Technical Guide* at [thermofisher.com](http://thermofisher.com) for detailed sample preparation procedures.
- Collect samples in pyrogen/endotoxin-free tubes.
- Freeze samples after collection if samples will not be tested immediately. Avoid multiple freeze-thaw cycles of frozen samples. Thaw completely and mix well (do not vortex) prior to analysis.
- Avoid the use of hemolyzed or lipemic sera. If large amounts of particulate matter are present in the sample, centrifuge or filter sample prior to analysis.

## Pre-dilute samples

Sample concentrations should be within the range of the standard curve. Because conditions may vary, each investigator should determine the optimal dilution for each application.


- Dilute samples with Standard Diluent Buffer.

## Dilute standards

**Note:** Use glass or plastic tubes for diluting standards.

**Note:** This assay has been calibrated against the WHO reference preparation 91/510 (NIBSC, Hertfordshire, UK, EN6 3QG). One microgram equals 1,700 International Units.

1. Reconstitute Hu IL-3 Standard to 10,000 pg/mL with Standard Dilution Buffer. Refer to the standard vial label for instructions. Swirl or mix gently and allow the contents to sit for 10 minutes to ensure complete reconstitution. Label as 10,000 pg/mL human IL-3. **Use the standard within 1 hour of reconstitution.**
2. Add 50  $\mu$ L Reconstituted Standard to one tube containing 950  $\mu$ L Standard Diluent Buffer and mix. Label as 500 pg/mL human IL-3.
3. Add 300  $\mu$ L Standard Diluent Buffer to each of 7 tubes labeled as follows: 250, 125, 62.5, 31.2, 15.6, 7.8 and 0 pg/mL human IL-3.
4. Make serial dilutions of the standard as shown in the following dilution diagram. Mix thoroughly between steps.
5. Remaining reconstituted standard should be discarded or frozen in aliquots at  $-80^{\circ}\text{C}$  for further use. Standard can be frozen and thawed one time only without loss of immunoreactivity.

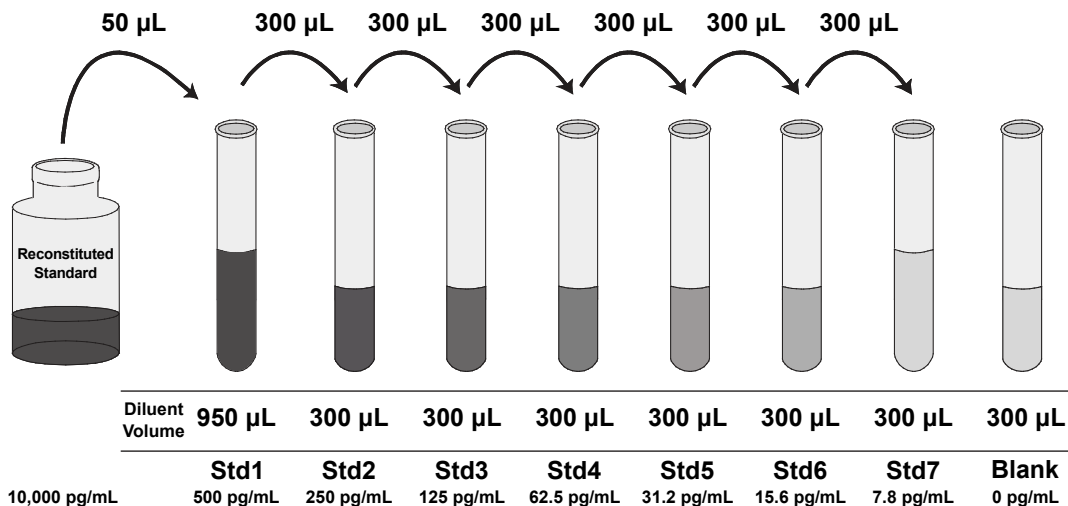

## Prepare 1X Streptavidin-HRP solution

**Note:** Prepare 1X Streptavidin-HRP within 15 minutes of usage.

The Streptavidin-HRP (100X) is in 50% glycerol, which is viscous. To ensure accurate dilution:






1. For each 8-well strip used in the assay, pipet 10  $\mu$ L Streptavidin-HRP (100X) solution, wipe the pipette tip with clean absorbent paper to remove any excess solution, and dispense the solution into a tube containing 1 mL of Streptavidin-HRP Diluent. Mix thoroughly.
2. Return the unused Streptavidin-HRP (100X) solution to the refrigerator.

## Perform ELISA (Total assay time: 4 hours)

**IMPORTANT!** Perform a standard curve with each assay.

- Allow all components to reach room temperature before use. Mix all liquid reagents prior to use.
- Determine the number of 8-well strips required for the assay. Insert the strips in the frames for use. Re-bag any unused strips and frames, and store at 2°C to 8°C for future use.



<b>1</b>	<b>Bind antigen</b> 	<ol style="list-style-type: none"> <li>Add 100 µL of standards, controls, or samples (see “Pre-dilute samples” on page 2) to the appropriate wells. Leave the wells for chromogen blanks empty.</li> <li>Cover the plate with a plate cover and incubate for 2 hours at room temperature.</li> <li>Thoroughly aspirate the solution and wash wells 4 times with 1X Wash Buffer.</li> </ol>
<b>2</b>	<b>Add Biotin Conjugate</b> 	<ol style="list-style-type: none"> <li>Add 100 µL Hu IL-3 Biotin Conjugate solution into each well except the chromogen blanks.</li> <li>Cover the plate with plate cover and incubate for 1 hour at room temperature .</li> <li>Thoroughly aspirate the solution and wash wells 4 times with 1X Wash Buffer.</li> </ol>
<b>3</b>	<b>Add Streptavidin-HRP</b> 	<ol style="list-style-type: none"> <li>Add 100 µL 1X Streptavidin-HRP solution (see page 2) into each well except the chromogen blanks.</li> <li>Cover the plate with a plate cover and incubate for 30 minutes at room temperature.</li> <li>Thoroughly aspirate the solution from the wells and wash wells 4 times with 1X Wash Buffer.</li> </ol>
<b>4</b>	<b>Add Stabilized Chromogen</b> 	<ol style="list-style-type: none"> <li>Add 100 µL Stabilized Chromogen to each well. The substrate solution begins to turn blue.</li> <li>Incubate for 30 minutes at room temperature in the dark.</li> </ol> <p><b>Note:</b> TMB should not touch aluminum foil or other metals.</p>
<b>5</b>	<b>Add Stop Solution</b> 	Add 100 µL Stop Solution to each well. Tap the side of the plate to mix. The solution in the wells changes from blue to yellow.

### Read the plate and generate the standard curve

1. Read the absorbance at 450 nm. Read the plate within 2 hours after adding the Stop Solution.
2. Use curve-fitting software to generate the standard curve. A four parameter algorithm provides the best standard curve fit. Optimally, the background absorbance may be subtracted from all data points, including standards, unknowns and controls, prior to plotting.
3. Read the concentrations for unknown samples and controls from the standard curve. Multiply value(s) obtained for sample(s) by the appropriate factor to correct for the sample dilution.

**Note:** Dilute samples producing signals greater than the upper limit of the standard curve in Standard Diluent Buffer and reanalyze. Multiply the concentration by the appropriate dilution factor.

### Performance characteristics

#### Standard curve example

The following data were obtained for the various standards over the range of 0 to 500 pg/mL human IL-3.

Standard Human IL-3 (pg/mL)	Optical Density (450 nm)
500	2.83
250	1.77
125	1.02
62.5	0.56
31.2	0.31
15.6	0.17
7.8	0.11
0	0.03

#### Inter-assay precision

Samples were assayed 42 times in multiple assays to determine precision between assays.

Parameters	Sample 1	Sample 2	Sample 3
Mean (pg/mL)	85.3	143.9	366.5
Standard Deviation	5.9	12.3	23.5
% Coefficient of Variation	6.9	8.6	6.4

#### Intra-assay precision

Samples of known human IL-3 concentration were assayed in replicates of 14 to determine precision within an assay.

Parameters	Sample 1	Sample 2	Sample 3
Mean (pg/mL)	87.2	152.8	362.4
Standard Deviation	4.6	8.9	19.8
% Coefficient of Variation	5.3	5.8	5.5

## Expected values

Ten sera and ten plasma (citrate) samples from apparently normal individuals were evaluated in this assay. The values for sera ranged from 0 to 4.8 pg/mL (mean 1.8 pg/mL). The values for plasma ranged from 0 to 85 pg/mL (mean 10 pg/mL).

Human PBMCs were cultured under the following conditions and the culture supernatants were assayed for human IL-3 released.

Sample	Hu IL-3 (pg/mL)
Unstimulated PBMC; 24 hr culture	1.4
PBMC + PMA (50 ng/mL), Ionophore (250 ng/mL); 24 hr culture	9,600
Unstimulated PBMC; 72 hr culture	12
PBMC + PMA (50 ng/mL), Ionophore (250 ng/mL); 72 hr culture	68,000

## Recovery

Sample	Average % Recovery
Serum	96
Plasma	93
Cell culture medium + 1% fetal bovine serum	123
Cell culture medium + 10% fetal bovine serum	113

## Limited product warranty

Life Technologies Corporation and/or its affiliate(s) warrant their products as set forth in the Life Technologies' General Terms and Conditions of Sale found on Life Technologies' website at [www.thermofisher.com/us/en/home/global/terms-and-conditions.html](http://www.thermofisher.com/us/en/home/global/terms-and-conditions.html). If you have any questions, please contact Life Technologies at [www.thermofisher.com/support](http://www.thermofisher.com/support).

## Linearity of dilution

Human serum and tissue culture medium containing 10% fetal bovine serum were spiked with human IL-3 and serially diluted in Standard Diluent Buffer over the range of the assay. Linear regression analysis of samples versus the expected concentration yielded a correlation coefficient of 0.99 in both cases.

Dilution	Serum			Cell Culture		
	Measured (pg/mL)	Expected (pg/mL) %		Measured (pg/mL)	Expected (pg/mL) %	
Neat	363	—	—	212	—	—
1/2	165	182	91	95	106	90
1/4	83	91	91	47	53	89
1/8	42	45	93	23	27	85
1/16	21	23	91	11	13	85
1/32	11	11	100	5.3	6.6	80








## Sensitivity

The analytical sensitivity of human IL-3 is <1 pg/mL. This was determined by adding two standard deviations to the mean O.D. obtained when the zero standard was assayed 30 times.

## Specificity

Buffered solutions of a panel of substances at 10,000 pg/mL were assayed with the Human IL-3 ELISA Kit. The following substances were tested and found to have no cross-reactivity: **human** IL-1 $\beta$ , IL-2, IL-4, IL-6, IL-7, IL-8, IL-10, IL-13, GM-CSF, IFN- $\gamma$ , TNF- $\alpha$ ; **mouse** IL-1 $\beta$ , IL-2, IL-3, IL-4, IL-6, IL-10, IFN- $\gamma$ , TNF- $\alpha$ ; **rat** TNF- $\alpha$ .

## Product label explanation of symbols and warnings

 REF	Catalog Number	 LOT	Batch code		Temperature limitation		Use by		Manufacturer		Consult instructions for use		Caution, consult accompanying documents
--	----------------	---	------------	---	------------------------	---	--------	---	--------------	---	------------------------------	---	---

**Manufacturer's address:** Life Technologies Corporation | 7335 Executive Way | Frederick, MD 21704 | USA

The information in this guide is subject to change without notice.

**DISCLAIMER:** TO THE EXTENT ALLOWED BY LAW, LIFE TECHNOLOGIES AND/OR ITS AFFILIATE(S) WILL NOT BE LIABLE FOR SPECIAL, INCIDENTAL, INDIRECT, PUNITIVE, MULTIPLE, OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH OR ARISING FROM THIS DOCUMENT, INCLUDING YOUR USE OF IT.

**Important Licensing Information:** These products may be covered by one or more Limited Use Label Licenses. By use of these products, you accept the terms and conditions of all applicable Limited Use Label Licenses.

**Corporate entity:** Life Technologies Corporation | Carlsbad, CA 92008 USA | Toll Free in USA 1 800 955 6288

©2017 Thermo Fisher Scientific Inc. All rights reserved. All trademarks are the property of Thermo Fisher Scientific and its subsidiaries unless otherwise specified.