


CaptureSelect™ hGH Ligand Leakage ELISA

Catalog Numbers 810316001 and 810316010

Pub. No. MAN0014057 Rev. A.0

Item	Description	Storage conditions
Coating reagent (green label)	Goat IgG anti-hGH affinity ligand, 100 µL	-20°C (-4°F)
Standard solution (blue label)	hGH affinity ligand, 100 µL	
Biotinylated reagent (yellow label)	Biotinylated Goat IgG anti-hGH affinity ligand, 100 µL	

 **WARNING!** Read the Safety Data Sheets (SDSs) and follow the handling instructions. Wear appropriate protective eyewear, clothing, and gloves. Safety Data Sheets (SDSs) are available from thermofisher.com/techresources.

Product description

The CaptureSelect™ hGH Ligand Leakage ELISA (Enzyme Linked Immuno-Sorbent Assay) is designed for the detection of 1 ng/mL hGH affinity ligand that may be present in product purified with CaptureSelect™ hGH affinity media, which contains the hGH affinity ligand as capturing agent. The assay is designed to minimize interference and to provide accurate quantitation in the presence of human growth hormone and other proteins. The hGH Ligand Leakage ELISA can be used as a tool to aid in optimal purification process development and in routine quality control of in-process streams as well as final product.

Principle of the assay

The CaptureSelect™ ligand leakage assay enables detection of the affinity ligand in solutions with and without the presence of the target protein. These sandwich assays involve the following steps:

- A microtiter plate is coated with affinity-purified anti-affinity ligand polyclonal goat antibodies.
- Samples containing the affinity ligand are incubated in the coated plate wells.
- Bound affinity ligand is detected by biotinylated affinity-purified anti-affinity ligand polyclonal goat antibodies.
- Streptavidin horseradish peroxidase conjugate is added to bind to the biotinylated antibody in the sandwich complex.
- Substrate reactive with horseradish peroxidase (tetramethylbenzidine-hydrogen peroxide) is added.
- The amount of hydrolyzed substrate is determined and is directly proportional to the concentration of affinity ligand present.

Required materials and equipment (not provided)

- PBS: Phosphate buffered saline pH 7.4
- PBST: Phosphate buffered saline (PBS) pH 7.4 + 0.05 (v/v)% Tween® 20 Solution
- Bovine Serum Albumin (BSA), Fraction V 99% pure (Sigma-Aldrich A3059)

Note: Other qualities of Bovine Serum Albumin or other blocking proteins might result in higher background levels.

- Dilution Buffer A: 0.05 (v/v)% Tween® 20 Solution in PBS pH 7.4
- 2X Dilution Buffer A: 0.1 (v/v)% Tween® 20 Solution in PBS pH 7.4
- Blocking solution: 4 (w/v)% BSA in PBS pH 7.4
- Streptavidin-Horseradish Peroxidase diluted immediately before using according to manufacturer guidelines

- Tetramethylbenzidine (TMB) and hydrogen peroxide (H₂O₂) substrate (prepare 1:1 solution immediately before use)
- 1 M H₂SO₄
- Microtiter plate (Maxisorp, Nunc)
- Microtiter plate shaker
- Microtiter plate reader (450 nm)
- Milli-Q® water

Procedure

Coat the plate

1. Make a 1:100 dilution of the Coating reagent with PBS pH 7.4.
2. Add 100 µL diluted Coating reagent to each well in a microtiter plate and incubate overnight at 4°C (39°F).

Prepare standards

1. Prepare a 6.4 µg/mL stock Standard solution: Add 10 µL Standard solution to 770 µL Dilution Buffer A.
2. Using the stock Standard solution from step 1, prepare a standard dilution series according to the table below.

Tube	Concentration (ng/mL)	Standard	Dilution Buffer A
1	64.0	10 µL diluted Standard solution	990 µL
2	16.0	250 µL 64.0 ng/mL	750 µL
3	8.0	500 µL 16.0 ng/mL	500 µL
4	4.0	500 µL 8.0 ng/mL	500 µL
5	2.0	500 µL 4.0 ng/mL	500 µL
6	1.0	500 µL 2.0 ng/mL	500 µL
7	0.5	500 µL 1.0 ng/mL	500 µL
8	0.25	500 µL 0.5 ng/mL	500 µL
9	0	0	500 µL

Prepare assay samples

Dilute 75 µL sample with 75 µL of 2X Dilution Buffer A.

ELISA assay procedure

1. Block the plate:
 - a. Wash the coated plate 5 times with PBST.
 - b. Add 200 µL/well of Blocking solution to the coated plate. Leave at room temperature for 30 minutes on a microtiter plate shaker.
 - c. Wash the plate 1 time with PBST.

2. Add samples and standards:
 - a. Add 100 μL of each concentration of the standard dilution series (0 to 64.0 ng/mL) or sample to appropriate wells.
 - b. Incubate the plate 1 hour at room temperature on a microtiter plate shaker.
 - c. Wash the plate 5 times with PBST.
3. Add Biotinylated reagents:
 - a. Make a 1:100 dilution of the Biotinylated reagents with Dilution Buffer A.
 - b. Add 100 μL diluted Biotinylated reagents to each well and incubate the plate 1 hour at room temperature.
 - c. Wash the plate 5 times with PBST.
4. Add diluted Streptavidin-Horseradish peroxidase:
 - a. Dilute in Dilution Buffer A according to the manufacturer's guidelines.
 - b. Add 100 μL diluted Streptavidin-Horseradish peroxidase to each well containing sample or standard.
 - c. Incubate the plate 1 hour at room temperature on a microtiter plate shaker.
 - d. Wash the plate 5 times with PBST.
 - e. Wash the plate 2 times with Milli-Q[®] water.
5. Develop and read the plate:
 - a. Add 100 μL 1:1 mixed TMB/H₂O₂ substrate per well.
 - b. Incubate the plate for approximately 15 minutes on a microtiter plate shaker.
 - c. When the background signal starts to develop, add 50 μL 1 M H₂SO₄ to stop the coloring reaction and achieve a maximal signal-to-noise ratio.
 - d. Measure the OD of the microtiter plate at 450 nm with a microtiter plate reader.

Calculate results

Construct a standard curve with values reported in ng/mL. Use curve-fitting routines such as 4-parameter logistic fit. Do not use linear regression analysis to interpolate values for samples, which may lead to significant inaccuracies.

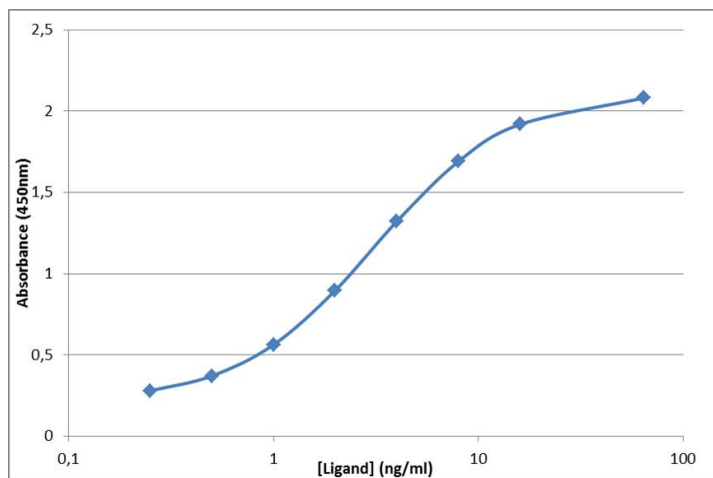


Figure 1 Example calibration curve hGH ligand leakage assay

Validate the assay

Perform validation studies that include at least the following experiments to validate this kit for your application: 1) Intra- and inter-assay precision experiments to establish reproducibility, 2) Recovery experiments using test samples with known amounts of the 500 $\mu\text{g/mL}$ Standard solution, which is included in the kit.

Ordering information

CaptureSelect™ hGH Ligand Leakage ELISA	Part number
1 assay	810316001
10 assays	810316010

For more information

For more information on CaptureSelect™ products and ligand leakage ELISA products, go to www.lifetechnologies.com/captureselect.

Customer and technical support

Visit thermofisher.com/techresources for the latest in services and support, including:

- Worldwide contact telephone numbers
- Product support, including:
 - Product FAQs
 - Software, patches, and updates
- Order and web support
- Product documentation, including:
 - User guides, manuals, and protocols
 - Certificates of Analysis
 - Safety Data Sheets (SDSs; also known as MSDSs)

Note: For SDSs for reagents and chemicals from other manufacturers, contact the manufacturer.

Limited product warranty

Life Technologies Corporation and/or its affiliate(s) warrant their products as set forth in the Life Technologies' General Terms and Conditions of Sale found on Life Technologies' website at www.lifetechnologies.com/termsandconditions. If you have any questions, please contact Life Technologies at www.lifetechnologies.com/support.

The information in this guide is subject to change without notice.

DISCLAIMER

TO THE EXTENT ALLOWED BY LAW, LIFE TECHNOLOGIES AND/OR ITS AFFILIATE(S) WILL NOT BE LIABLE FOR SPECIAL, INCIDENTAL, INDIRECT, PUNITIVE, MULTIPLE, OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH OR ARISING FROM THIS DOCUMENT, INCLUDING YOUR USE OF IT.

Important Licensing Information: These products may be covered by one or more Limited Use Label Licenses. By use of these products, you accept the terms and conditions of all applicable Limited Use Label Licenses.

©2015 Thermo Fisher Scientific Inc. All rights reserved. All trademarks are the property of Thermo Fisher Scientific and its subsidiaries unless otherwise specified. Tween is a registered trademark of Uniqema Americas, LLC. Milli-Q is a registered trademark of Merck KGaA.

For support visit thermofisher.com/techresources or email techsupport@lifetech.com

lifetechnologies.com