


Human Cytokine Magnetic 30-Plex Panel Technical Data Sheet

Performance Characteristics

Typical Standard Curves (Note: Data presented here were collected as a 30-plex, but are depicted in 5-plex groupings for clarity.)

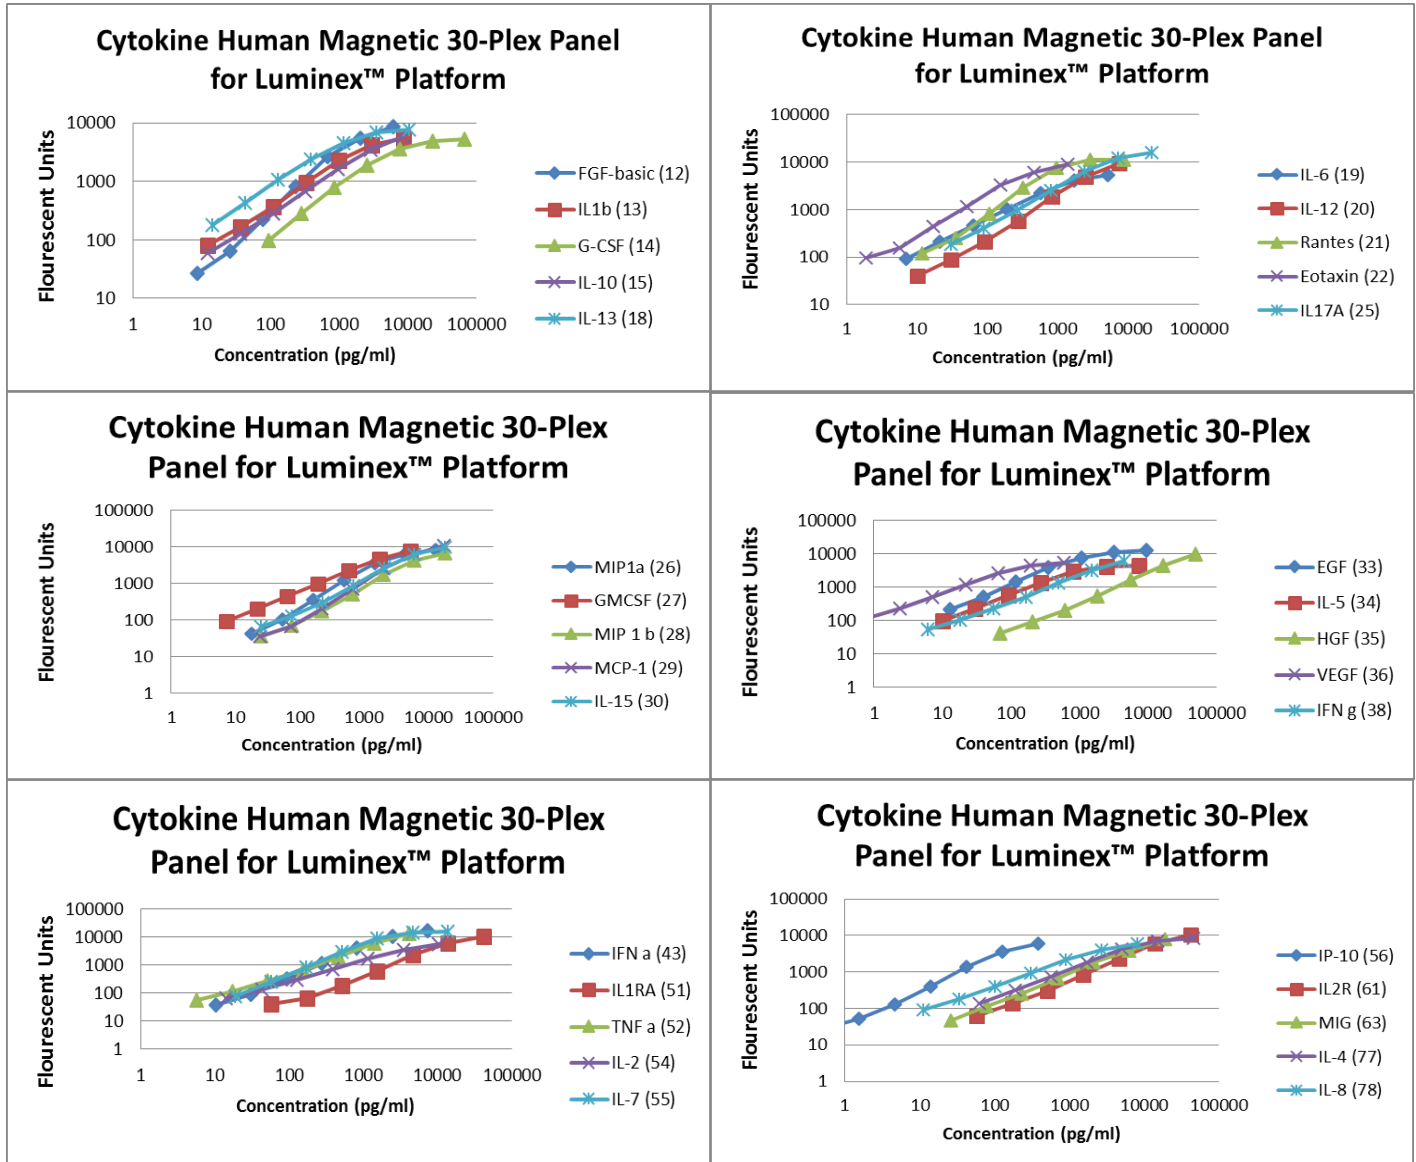

Analyte	Magnetic Bead Region	Sensitivity (pg / mL)	Recovery					NIBSC calibration	NIBSC Preparation Number	Intra assay CV*
			Serum	EDTA Plasma	Citrate Plasma	Heparin Plasma	TC*			
EGF	33	<5	√	√	√	√	√	N/A	N/A	4.0 %
Eotaxin	22	<0.5	√	√	√	NR	√	N/A	N/A	9.0 %
FGF-basic	12	<10	√	√	-	NR	√	N/A	N/A	3.0 %
G-CSF	14	<15	NR	NR	NR	NR	√	N/A	N/A	2.4 %
GM-CSF	27	<0.5	√	√	√	√	√	1 ng = 6 IU	88/646	9.1 %
HGF	35	<10	√	√	√	NR	√	N/A	N/A	4.7 %
IFN alpha	43	<5	√	-	√	√	√	1 ng = 14 IU	94/784	7.9 %
IFN gamma	38	<0.5	√	√	√	-	√	1 ng = 0.7 IU	82/587	9.0 %
IL-10	15	<0.5	√	√	√	√	√	1 ng = 13 IU	93/722	9.8 %
IL-12	20	<1	√	√	√	-	√	1 ng = 11 IU	95/544	8.1 %
IL-13	18	<1	√	√	√	√	√	1 ng = 1.2 IU	94/622	9.6 %
IL-15	30	<5	√	√	√	√	√	1 ng = 150 IU	95/554	7.6 %
IL-17A	25	<1	√	√	√	√	√	1 ng = 10 IU	01/420	6.0 %
IL-1 beta	13	<5	√	√	√	√	√	1 ng = 25 IU	86/680	8.8 %
IL-1RA	51	<10	√	√	√	√	√	1 ng =0.001 ImU	92/644	5.1 %
IL-2	54	<0.5	√	√	√	√	√	1 ng = 7 IU	86/564	9.6 %
IL-2R	61	<10	√	√	√	√	√	1 ng = 12.2-40.6 IU	97/600	4.2 %
IL-4	77	<5	√	√	√	√	√	1 ng = 65 IU	88/656	8.7 %
IL-5	34	<0.5	√	√	√	√	√	1 ng =0.2 IU	90/586	7.5 %
IL-6	19	<0.5	√	√	√	√	√	1 ng =30 IU	89/548	7.0 %
IL-7	55	<5	√	√	√	NR	√	1 ng = 64 IU	90/530	9.8 %
IL-8	78	<1	√	√	√	√	√	1 ng = 40 IU	89/520	9.8 %
IP-10	56	<0.5	√	√	√	√	√	N/A	N/A	3.7 %
MCP-1	29	<5	√	√	√	√	√	1 ng= 1.5 IU	92/794	5.8 %
MIG	63	<5	√	√	√	NR	√	N/A	N/A	9.4 %
MIP-1 beta	28	<5	√	√	√	√	√	N/A	N/A	3.6 %
MIP-1 alpha	26	<5	√	√	√	√	√	1 ng = 0.4 IU	92/518	9.5 %
Rantes**	21	<5	√	√	√	√	√	1 ng = 0.7 IU	92/520	8.9 %
TNF alpha	52	<0.5	√	√	√	√	√	1 ng = 0.2 IU	88/786	8.3 %
VEGF	36	<0.5	√	√	√	√	√	N/A	N/A	4.8 %

*Analysis performed during product development and with first lots produced.

**Additional sample dilution required for accurate recovery.

Notes: 70-130% recovery (√), 50-69% recovery (-), 131-150% recovery (+), <50% or >150% recovery (NR - not recommended)

Limited product warranty

Life Technologies Corporation and/or its affiliate(s) warrant their products as set forth in the Life Technologies' General Terms and Conditions of Sale found on Life Technologies' website at www.thermofisher.com/us/en/home/global/terms-and-conditions.html. If you have any questions, please contact Life Technologies at www.thermofisher.com/support.

Product label explanation of symbols and warnings

REF	Catalog Number	LOT	Batch code	Temperature limitation	Use by	Manufacturer	Consult instructions for use	Caution, consult accompanying documents
-----	----------------	-----	------------	------------------------	--------	--------------	------------------------------	---

Manufacturer's address: Bender MedSystems GmbH | Campus Vienna Biocenter 2 | 1030 Vienna, Austria

The information in this guide is subject to change without notice.

DISCLAIMER: TO THE EXTENT ALLOWED BY LAW, LIFE TECHNOLOGIES AND/OR ITS AFFILIATE(S) WILL NOT BE LIABLE FOR SPECIAL, INCIDENTAL, INDIRECT, PUNITIVE, MULTIPLE, OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH OR ARISING FROM THIS DOCUMENT, INCLUDING YOUR USE OF IT.

Important Licensing Information: These products may be covered by one or more Limited Use Label Licenses. By use of these products, you accept the terms and conditions of all applicable Limited Use Label Licenses.

©2018 Thermo Fisher Scientific Inc. All rights reserved. All trademarks are the property of Thermo Fisher Scientific and its subsidiaries unless otherwise specified.

For Research Use Only. Not for use in diagnostic procedures.

MAN0017761 Rev. A.0 (00) Effective Date:21 March 2018

Manufacturing site: Bender MedSystems GmbH | Campus Vienna Biocenter 2 | 1030 Vienna, Austria