

Mouse Adiponectin ELISA Kit

Catalog Number KMP0041 (96 tests)

Pub. No. MAN0004522 Rev. 6.0 (30)

CAUTION! This kit contains materials with small quantities of Proclin™ 300. Proclin™ 300 is toxic, corrosive, and a skin irritant. Avoid ingestion and contact with eyes, skin and mucous membranes. Observe all federal, state, and local regulations for disposal.

Note: For safety and biohazard guidelines, see the “Safety” appendix in the *ELISA Technical Guide* (Pub. no. MAN0006706). Read the Safety Data Sheets (SDSs) and follow the handling instructions. Wear appropriate protective eyewear, clothing, and gloves.

Product description

The Invitrogen™ Mouse Adiponectin ELISA Kit is a solid-phase sandwich Enzyme-Linked Immunosorbent Assay (ELISA). This assay is designed to detect and quantify the level of mouse adiponectin in serum, plasma, and cell culture supernatants. The assay will recognize both natural and recombinant mouse adiponectin.

Adiponectin is an adipocyte-specific protein and represents a major serum protein. The full length adiponectin in plasma exists as trimer, hexamer, and multimer. Extremely low amounts of the globular domain also exist in plasma as trimer.

Contents and storage

Upon receipt, store the kit at 2°C to 8°C.

Contents	Cat. No. KMP0041 (96 tests)
Ms Adiponectin Standard, lyophilized	1 vial
Antibody Coated Wells, 96-well plate	1 plate
Ms Adiponectin Detection Antibody 200X	60 µL
Anti-Rabbit IgG HRP 100X	150 µL
ELISA Buffer (10X)	2 × 30 mL
Wash Buffer (10X)	2 × 30 mL
TMB Substrate Solution	12 mL
Stop Solution	12 mL
Adhesive Plate Covers	2

Materials required but not supplied

- Distilled or deionized water
- Calibrated adjustable precision pipettes and glass or plastic tubes for diluting solutions; beakers, flask and cylinders for preparation of reagents
- Microtiter plate reader with software capable of measurement at or near 450 nm
- Plate washer—automated or manual (squirt bottle, manifold dispenser, or equivalent)

Before you begin

IMPORTANT! Reagents are lot-specific. Do not mix or interchange different reagent lots from various kit lots.

- Review the **Procedural guidelines** and **Plate washing directions** in the *ELISA Technical Guide* available at thermofisher.com.
- Allow reagents to reach room temperature before use. Mix to redissolve any precipitated salts.

Prepare 1X Wash Buffer

1. Dilute 30 mL of Wash Buffer Concentrate (10X) with 270 mL of deionized or distilled water. Label as 1X Wash Buffer.
2. Store the concentrate and 1X Wash Buffer in the refrigerator. Use the diluted buffer within 14 days.

Sample preparation guidelines

- Refer to the *ELISA Technical Guide* at thermofisher.com for detailed sample preparation procedures.
- Collect samples in pyrogen/endotoxin-free tubes.
- Freeze samples after collection if samples will not be tested immediately. Avoid multiple freeze-thaw cycles of frozen samples. Thaw completely and mix well (do not vortex) prior to analysis.
- Avoid the use of hemolyzed or lipemic sera. If large amounts of particulate matter are present in the sample, centrifuge or filter sample prior to analysis.

Pre-dilute samples

Sample concentrations should be within the range of the standard curve. Because conditions may vary, each investigator should determine the optimal dilution for each application.

- Perform sample dilutions with 1X ELISA Buffer.
- Dilute **serum** and **plasma** samples 20,000-fold.


Prepare 1X ELISA Buffer

Dilute 10X ELISA Buffer 1:10 (e.g., 20 mL 10X ELISA Buffer with 180 mL of deionized water). Label as 1X ELISA Buffer.

Dilute standards

Note: Use glass or plastic tubes for diluting standards.

1. Reconstitute Ms Adiponectin Standard to 16 ng/mL with 1 mL of deionized water. Swirl or mix gently and allow the contents to sit for 10 minutes to ensure complete reconstitution. Label as 16 ng/mL mouse adiponectin. **Use the standard within 1 hour of reconstitution.**
2. Add 300 μ L 1X ELISA Buffer to each of 8 tubes labeled as follows: 8, 4, 2, 1, 0.5, 0.25, 0.125, and 0 ng/mL mouse adiponectin.
3. Make serial dilutions of the standard as shown in the following dilution diagram. Mix thoroughly between steps.
4. Discard any remaining reconstituted standard.

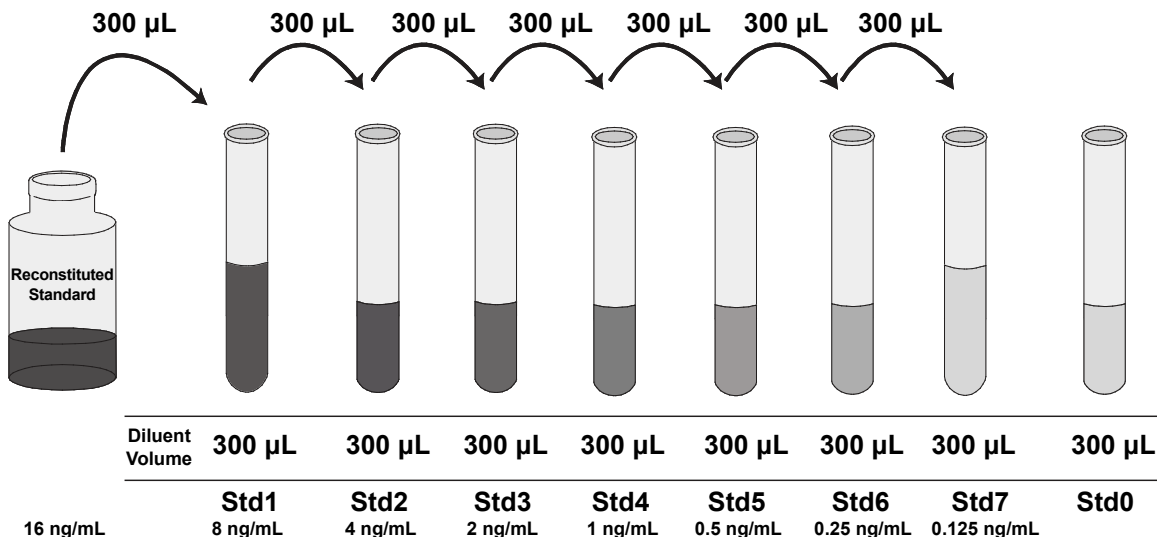

Prepare 1X Detection Antibody solution

Dilute 50 μ L of Detection Antibody 200X with 10 mL of 1X ELISA Buffer. Label as 1X Detector Antibody.

Note: The diluted Detection Antibody is not stable and cannot be stored.

Prepare 1X Anti-Rabbit IgG HRP solution

Note: Prepare 1X Anti-Rabbit IgG HRP solution within 1 hour of usage.






Dilute HRP 100X 1:100. Add 100 μ L to 10 mL of 1X ELISA Buffer. Label as 1X HRP solution

Perform ELISA (Total assay time: 3.5 hours)

IMPORTANT! Perform a standard curve with each assay.

- Allow all components to reach room temperature before use. Mix all liquid reagents prior to use.
- Determine the number of 8-well strips required for the assay. Insert the strips in the frames for use. Re-bag any unused strips and frames, and store at 2°C to 8°C for future use.



1	Bind antigen 	<ol style="list-style-type: none"> Add 100 µL of standards, controls, or samples (see "Pre-dilute samples" on page 2) to the appropriate wells. Leave the wells for chromogen blanks empty. Cover the plate with a plate cover and incubate 1 hour at 37°C. Thoroughly aspirate the solution and wash wells 3 times with 1X Wash Buffer.
2	Add detector antibody 	<ol style="list-style-type: none"> Add 100 µL of Ms Adiponectin Detection Antibody solution into each well except the chromogen blanks. Cover the plate with a plate cover and incubate 1 hour at 37°C. Thoroughly aspirate the solution and wash wells 3 times with 1X Wash Buffer.
3	Add IgG HRP 	<ol style="list-style-type: none"> Add 100 µL Anti-Rabbit IgG HRP into each well except the chromogen blanks. Cover the plate with plate cover and incubate for 1 hour at 37°C. Thoroughly aspirate the solution and wash wells 5 times with 1X Wash Buffer.
4	Add TMB Substrate Solution 	<ol style="list-style-type: none"> Add 100 µL TMB Substrate Solution to each well. The substrate solution begins to turn blue. Incubate for 20 minutes at room temperature in the dark. <p>Note: TMB should not touch aluminum foil or other metals.</p>
5	Add Stop Solution 	Add 100 µL Stop Solution to each well. Tap the side of the plate to mix. The solution in the wells changes from blue to yellow.

Read the plate and generate the standard curve

1. Read the absorbance at 450 nm. Read the plate within 30 minutes after adding the Stop Solution.
2. Use curve-fitting software to generate the standard curve. A 4 parameter algorithm provides the best standard curve fit. Optimally, the background absorbance may be subtracted from all data points, including standards, unknowns and controls, prior to plotting.
3. Read the concentrations for unknown samples and controls from the standard curve. Multiply value(s) obtained for sample(s) by the appropriate factor to correct for the sample dilution.


Note: Dilute samples producing signals greater than the upper limit of the standard curve in 1X ELISA Buffer and reanalyze. Multiply the concentration by the appropriate dilution factor.

Performance characteristics

Standard curve example

Typical standard curve over the range of 0 to 8 ng/mL mouse adiponectin.

Standard Mouse Adiponectin (ng/mL)	Optical Density (450 nm)
8	2.38
4	1.51
2	0.88
1	0.45
0.5	0.24
0.25	0.13
0.125	0.06
0	0

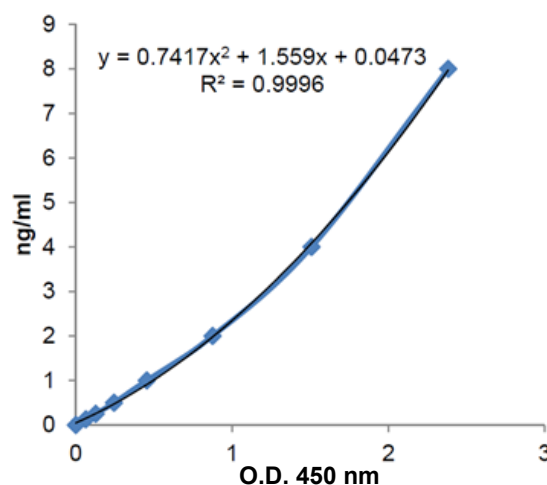

Inter-assay precision

Five samples of known mouse adiponectin concentration were assayed in replicates of 10 to determine precision between assays.

Parameters	Sample 1	Sample 2	Sample 3	Sample 4	Sample 5
Mean (µg/mL)	18.01	15.07	18.78	15.95	16.17
Standard Deviation	0.49	1.00	0.79	1.26	0.78
% Coefficient of Variation	2.71	6.62	4.19	7.88	4.80

Intra-assay precision

Five samples of known mouse adiponectin concentration were assayed in replicates of 10 to determine precision within an assay.

Parameters	Sample 1	Sample 2	Sample 3	Sample 4	Sample 5
Mean (µg/mL)	19.16	15.52	23.99	17.62	17.19
Standard Deviation	0.37	0.64	0.35	0.43	0.56
% Coefficient of Variation	1.91	4.15	1.44	2.45	3.23

Expected values

The levels for mouse adiponectin in plasma and serum range from 10 to >80 µg/mL (from normal mice).

Sensitivity

The analytical sensitivity of the assay is 50 pg/mL mouse adiponectin.

Specificity

This ELISA is specific for the measurement of natural and recombinant mouse adiponectin. It does not cross-react with **Human** Adiponectin or TNF-α; **Rat** Adiponectin; **Mouse** resistin, RELM-β or leptin.

Limited product warranty

Life Technologies Corporation and/or its affiliate(s) warrant their products as set forth in the Life Technologies' General Terms and Conditions of Sale found on Life Technologies' website at www.thermofisher.com/us/en/home/global/terms-and-conditions.html. If you have any questions, please contact Life Technologies at www.thermofisher.com/support.

Linearity of dilution

Different mouse serum samples containing mouse adiponectin were diluted several fold (1:20,000 to 1:40,000).








Samples	Sample Dilution	Expected (µg/mL)	Observed (µg/mL)	% of Expected
1	1:20,000	33.18	33.18	100.0
	1:30,000	22.12	24.44	110.5
	1:40,000	16.59	17.06	102.8
2	1:20,000	40.47	40.47	100.0
	1:30,000	26.98	26.94	99.8
	1:40,000	20.24	21.75	107.5
3	1:20,000	52.48	52.48	100.0
	1:30,000	34.98	32.88	94.0
	1:40,000	26.24	26.92	102.6

Recovery

When serum samples are spiked with known concentrations of mouse adiponectin, the recovery averages 97% (range 91 to 105%).

Sample	Average % Recovery	% Range
1	102.2	98-105
2	96.0	93-98
3	96.0	91-98
4	95.0	92-97
5	98.0	93-102

Product label explanation of symbols and warnings

 REF	Catalog Number	 LOT	Batch code		Temperature limitation		Use by		Manufacturer		Consult instructions for use		Caution, consult accompanying documents
--	----------------	---	------------	---	------------------------	---	--------	---	--------------	---	------------------------------	---	---

Manufacturer's address: Bender MedSystems GmbH | Campus Vienna Biocenter 2 | 1030 Vienna, Austria

The information in this guide is subject to change without notice.

DISCLAIMER: TO THE EXTENT ALLOWED BY LAW, LIFE TECHNOLOGIES AND/OR ITS AFFILIATE(S) WILL NOT BE LIABLE FOR SPECIAL, INCIDENTAL, INDIRECT, PUNITIVE, MULTIPLE, OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH OR ARISING FROM THIS DOCUMENT, INCLUDING YOUR USE OF IT.

Important Licensing Information: These products may be covered by one or more Limited Use Label Licenses. By use of these products, you accept the terms and conditions of all applicable Limited Use Label Licenses.

©2018 Thermo Fisher Scientific Inc. All rights reserved. All trademarks are the property of Thermo Fisher Scientific and its subsidiaries unless otherwise specified.