

# ProcartaPlex™ Human Coagulation Panel 3 4-Plex

## USER GUIDE

**Catalog Number** EPX040-10825-901

**Publication Number** MAN0024717

**Revision** A.0 (30)



Bender MedSystems GmbH | Campus Vienna Biocenter 2 | 1030 Vienna, Austria

For descriptions of symbols on product labels or product documents, go to [thermofisher.com/symbols-definition](https://www.thermofisher.com/symbols-definition).

The information in this guide is subject to change without notice.

**DISCLAIMER:** TO THE EXTENT ALLOWED BY LAW, THERMO FISHER SCIENTIFIC INC. AND/OR ITS AFFILIATE(S) WILL NOT BE LIABLE FOR SPECIAL, INCIDENTAL, INDIRECT, PUNITIVE, MULTIPLE, OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH OR ARISING FROM THIS DOCUMENT, INCLUDING YOUR USE OF IT.

**End User License Agreement for Luminex Assay Products:** By opening the packaging containing this Assay Product (which contains fluorescently labeled microsphere beads authorized by Luminex Corporation) or using this Assay Product in any manner, you are consenting and agreeing to be bound by the End User Terms and Conditions and the End User License Agreement available at <https://www.luminexcorp.com/end-user-terms-and-conditions/#sec3>. If you do not agree to all of the terms and conditions, you must promptly return this Assay Product for a full refund prior to using it in any manner.

**Revision history:** Pub. No. MAN0024717

Revision	Date	Description
A.0 (30)	23 February 2021	new manual

**TRADEMARKS:** xMAP, Luminex 100/200, MAGPIX, INTELLIFLEX and FLEXMAP 3D are trademarks of Luminex Corp. and Bio-Plex is a trademark of Bio-Rad Laboratories Inc. All trademarks are the property of Thermo Fisher Scientific and its subsidiaries unless otherwise specified.

©2021 Thermo Fisher Scientific Inc. All rights reserved.

# Contents

■	<b>CHAPTER 1</b>	<b>ProcartaPlex™ Human Coagulation Panel 3 4-Plex</b>	<b>4</b>
		Introduction	4
		Contents and storage	5
		Required materials not supplied	5
		Precautions and technical hints	6
		Workflow	7
■	<b>CHAPTER 2</b>	<b>Methods</b>	<b>8</b>
		Sample preparation	8
		Plasma sample preparation	8
		Dilution of plasma samples	8
		Preparation of reagents	8
		Prepare 1X Wash Buffer	9
		Prepare 1X Universal Assay Buffer (UAB)	9
		Prepare 1X Detection Antibody Mix	9
		Prepare Control Plasma	9
		Prepare 4-fold serial dilution	10
		Assay protocol	11
		Instrument settings	13
		Analyze results	13
■	<b>APPENDIX A</b>	<b>Recommended plate layout</b>	<b>14</b>



# ProcartaPlex™ Human Coagulation Panel 3 4-Plex



**WARNING!** Read the Safety Data Sheets (SDSs) and follow the handling instructions. Wear appropriate protective eyewear, clothing, and gloves. Safety Data Sheets (SDSs) are available from [thermofisher.com/support](https://www.thermofisher.com/support).

## Introduction

The ProcartaPlex™ Coagulation Panel 3 4-Plex has been optimized for detection of multiple analytes from EDTA and citrate plasma.

The panel is provided with individual vials of 1X capture and 50X detection reagents and is not combinable with simplex or other panels.

ProcartaPlex™ preconfigured panels are extensively tested for analyte combinability, interference and cross-reactivity to provide the highest level of validation and precision. All ProcartaPlex™ panels are supplied with the necessary reagents to perform the assay.

Analytes		
Factor IX	Protein C	Protein S
vWF		

For detailed product information, visit [thermofisher.com/procartaplex](https://www.thermofisher.com/procartaplex)

## Contents and storage

Upon receipt, store the kit at 2°C to 8°C. When stored as indicated, all reagents are stable until the expiration date.

Contents	Amount
Control Plasma	2 each
Biotinylated Detection Antibody (50X)	1 x 70 µL
Capture Bead Mix (1X)	1 x 5 mL
Streptavidin-PE (SA-PE) (1X)	1 x 5 mL
Wash Buffer (10X)	1 x 25 mL
Reading Buffer (1X)	1 x 40 mL
Universal Assay Buffer (10X)	1 x 10 mL
Detection Antibody Diluent (1X)	1 x 3 mL
8-Tube Strip	2 each
Flat Bottom 96-well Plate, black	1 each
Microplate Lid	1 each
Plate Seals	8 each

Retain the lot-specific Certificate of Analysis that contains the product expiration date. The Certificate of Analysis also contains important information such as bead number, analyte names and highest Control Plasma concentration required for the assay setup on the xMAP instrument.



**CAUTION!** This kit contains materials with small quantities of sodium azide. Sodium azide reacts with lead and copper plumbing to form explosive metal azides. Upon disposal, flush drains with a large volume of water to prevent azide accumulation. Avoid ingestion and contact with eyes, skin and mucous membranes. In case of contact, rinse affected area with plenty of water. Observe all federal, state and local regulations for disposal.

## Required materials not supplied

- xMAP™ instrument
- Hand-Held Magnetic Plate Washer (Cat. No. EPX-55555-000)
- Deionized water
- Vortex mixer (e.g., Cat. No. 88882010)
- Microcentrifuge
- Adjustable single and multichannel pipettes with disposable tips and low volume reservoirs (e.g., Cat. No. 95128093)

- Beakers, flasks, and cylinders necessary for preparation of reagents
- Orbital microplate shaker with at least 1.5 mm or 0.059 inch orbit diameter capable of maintaining a speed of  $600 \pm 50$  rpm (e.g., Cat. No. 88882006)

---


**Note:** The use of rockers or large orbit shakers may cause adverse results.

---

## Precautions and technical hints

1. Thoroughly read this User Guide and Certificate of Analysis prior to using the kit.
2. All chemicals should be considered potentially hazardous.
3. To avoid cross-contamination, do not invert the assay plate during the assay or allow contents from one well to mix with another well.
4. Use a multichannel pipette and reagent reservoirs whenever possible to achieve optimal assay precision.
5. Ensure that the xMAP™ instrument has been properly calibrated and set up prior to preparing and running the assay.

## Workflow

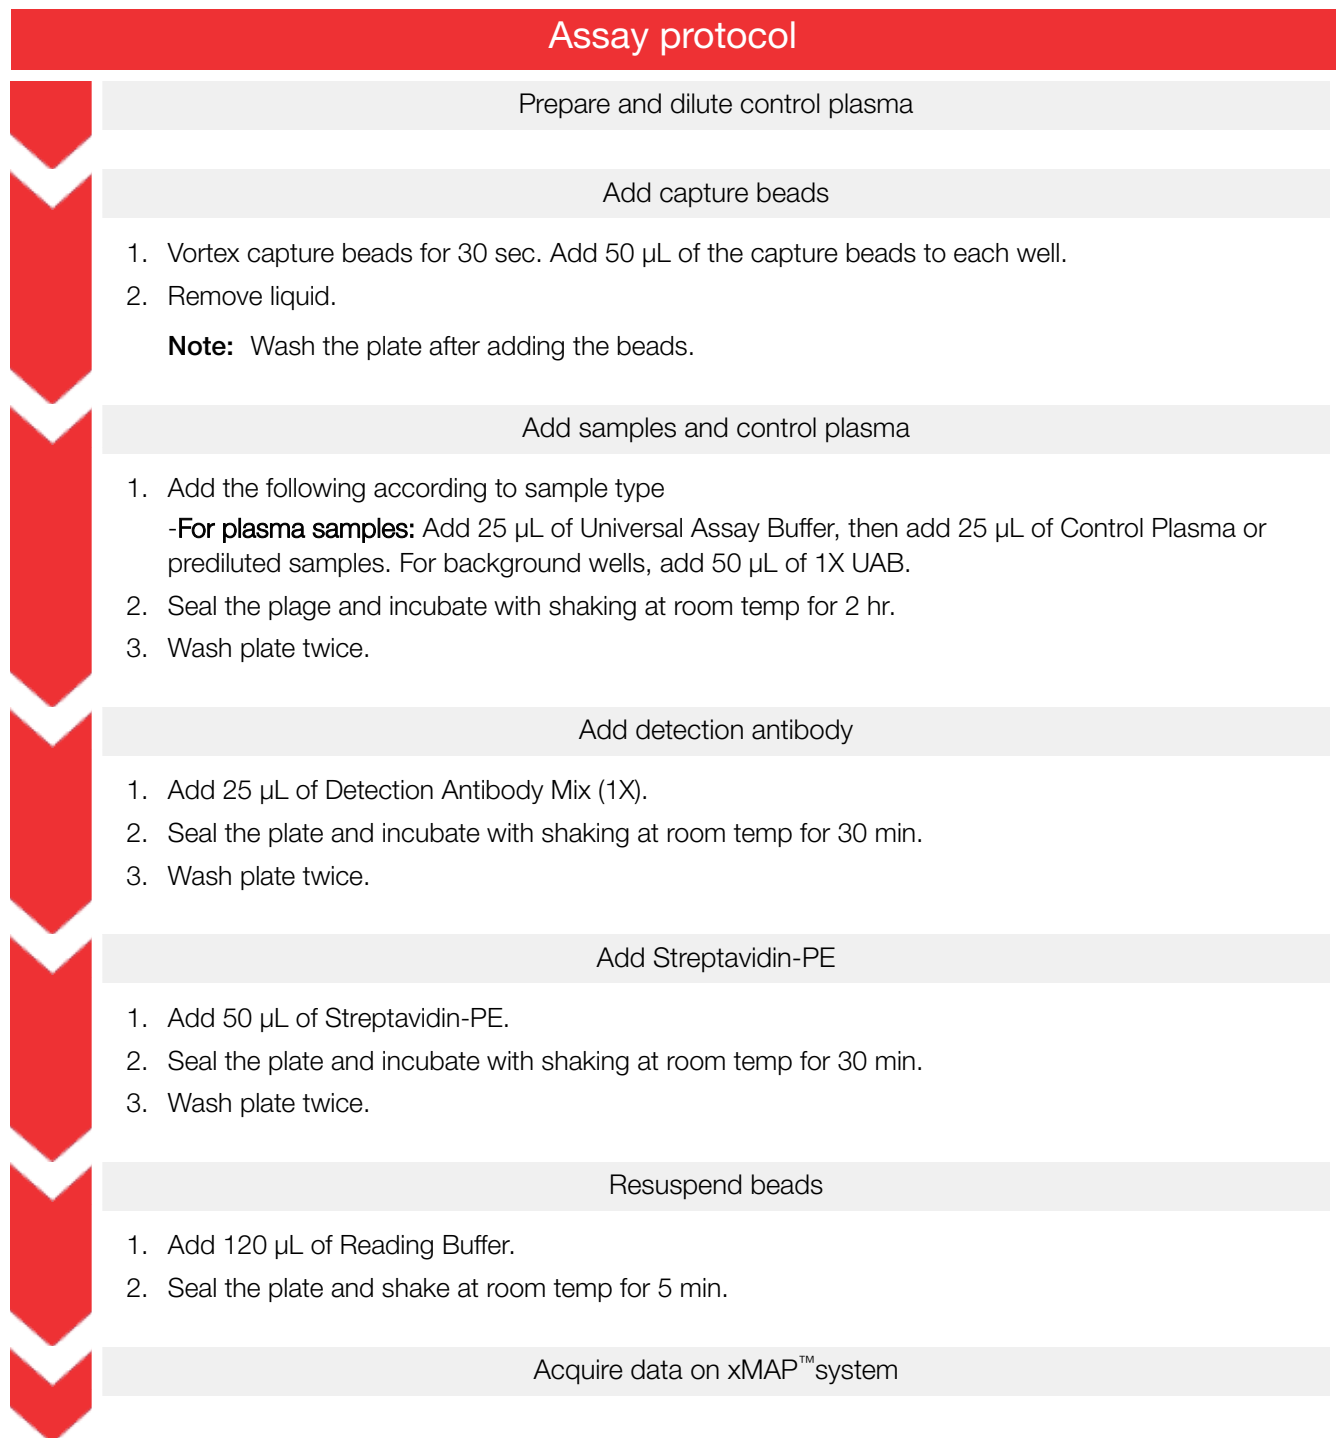

## Sample preparation

Thaw frozen plasma samples on ice and mix well by vortexing. Centrifuge at  $10,000 \times g$  for 5–10 minutes to pellet out particulates. Avoid multiple freeze/thaw cycles. If samples are high in lipid content, centrifuge at  $10,000 \times g$  for 10 minutes and transfer contents to a new tube.

### Plasma sample preparation

1. Collect samples in sodium citrate or EDTA tubes.
2. Centrifuge samples at  $1,000 \times g$  at  $4^{\circ}\text{C}$  for 10 minutes within 30 minutes of collection.
3. Collect the plasma fraction. Use immediately or store aliquots at  $-80^{\circ}\text{C}$ .

### Dilution of plasma samples

The analytes included in the panel typically have high plasma concentrations. We recommend that you dilute samples 1:500 in 1X Universal Assay Buffer (UAB) to ensure that they fall within range of the assay. To prepare 1X UAB, “Prepare 1X Universal Assay Buffer (UAB)” on page 9.

Tube	Sample volume	Assay diluent volume
Dilution 1 (1:50)	10 $\mu\text{L}$	490 $\mu\text{L}$
Dilution 2 (1:10)	10 $\mu\text{L}$ of Dilution 1	90 $\mu\text{L}$

## Preparation of reagents

Before starting with the assay protocol, define the plate map. Mark the Control Plasma, sample and background wells using the plate map found in Appendix A, “Recommended plate layout” to determine the number of wells used.



## Prepare 1X Wash Buffer

Bring the Wash Buffer Concentrate (10X) to room temperature and vortex for 15 seconds. Mix 20 mL of the Wash Buffer Concentrate (10X) with 180 mL ddH<sub>2</sub>O. Mix gently to avoid foaming. Wash Buffer (1X) can be stored at 2–8°C for up to 6 months.

---

**Note:** Additional Wash Buffer Concentrate (200 mL, Cat. No. EPX-66666-001) can be purchased separately for automated plate washers.

---

## Prepare 1X Universal Assay Buffer (UAB)

---

**Note:** 1X UAB is required for the preparation of Control Plasma and dilution of plasma samples.

---

Mix 10 mL of 10X Universal Assay Buffer (UAB) with 90 mL ddH<sub>2</sub>O. Mix gently to avoid foaming. 1X UAB can be stored at 2° to 8 °C for up to 30 days.

## Prepare 1X Detection Antibody Mix

Detection antibody is provided at a 50X concentration and requires dilution prior to use. The steps below provide diluted detection antibody mix for a 96-well plate.

1. Add 60 µL of the detection antibody concentrate to the mixing bottle.
2. Add Detection Antibody Diluent (1X) to a final volume of 3 mL if using the entire 96-well plate (otherwise adjust the volume accordingly).

## Prepare Control Plasma

This kit is supplied with one lyophilized Control Plasma for generation of standard curves. Two vials of the Control Plasma are provided to permit the user to run the assay twice if running a partial plate. Use 1X UAB as the diluent to reconstitute and dilute the Control Plasma.

---

**Note:** Change pipette tips after each dilution step and avoid air bubbles.

---

1. Centrifuge the Control Plasma stock vial at 2,000 x g for 10 seconds.
2. Add 250 µL of diluent to the stock vial.
3. Vortex the vial at high speed for 30 seconds and centrifuge at 2,000 x g for 10 seconds to collect contents at the bottom of the vial.
4. Incubate on ice for 10 minutes to ensure complete reconstitution.
5. Dilute the Control Plasma 1:40 by adding 25 µL of the previously prepared Control Plasma to 975 µL Universal Assay Buffer (1X).


## Prepare 4-fold serial dilution

1. Label the tubes in the 8-Tube Strip: Std1, Std2, Std3, Std4, Std5, Std6 and Std7.
2. Add 200  $\mu\text{L}$  of the reconstituted and diluted Control Plasma into Std1 tube.
3. Add 150  $\mu\text{L}$  of diluent into Std2–Std7 tubes.
4. Transfer 50  $\mu\text{L}$  from Std1 tube into Std2 tube.
5. Mix by pipetting up and down 10 times.
6. Transfer 50  $\mu\text{L}$  of the mixed Control Plasma from Std2 tube into Std3 tube using new pipette tip.
7. Mix by pipetting up and down 10 times.
8. Repeat steps 4–7 for tubes Std4–Std7, changing pipette tips between dilution steps.
9. Add 150  $\mu\text{L}$  of diluent to the last tube of the 8-Tube Strip to serve as a background.
10. Keep tubes on ice until ready to use.

---

**Note:** Use the reconstituted Control Plasma immediately. The reconstituted Control Plasma cannot be stored. Discard unopened Control Plasma vials if the entire plate was used in a single experiment.

---

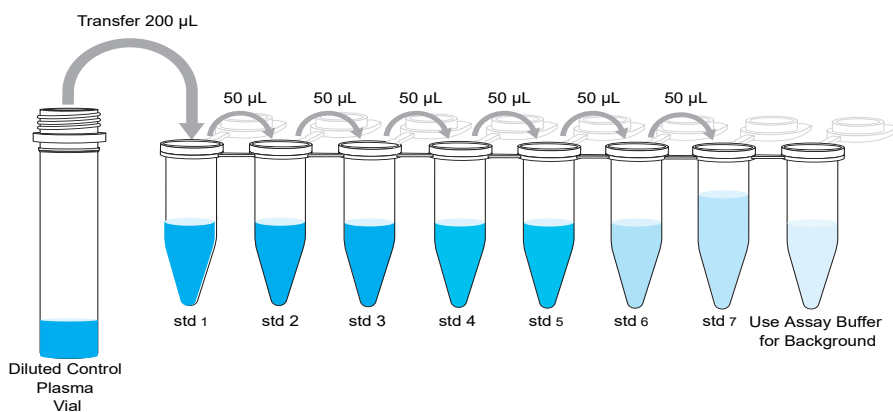

## Assay protocol

1. Add Capture Bead Mix to the plate.
  - a. Vortex the 1X Capture Bead Mix vial for 30 seconds at high speed.
  - b. Using a multichannel pipette, add 50  $\mu$ L of the Capture Bead Mix to each well of the plate.
2. Wash beads using a Hand-Held Magnetic Plate Washer.

---

**Note:** To avoid loss of beads, secure the plate using the clamps on both sides of the Hand-Held Magnetic Plate Washer during this procedure.

---

---

**Note:** This protocol was developed using the Hand-Held Magnetic Plate Washer (Cat. No. EPX-55555-000). Other washers should be validated by the end user.

---

- a. Place the plate on the Hand-Held Magnetic Plate Washer and wait 2 minutes to allow the beads to settle on the bottom of each well.
  - b. Remove the liquid by quickly inverting the washer/plate assembly over a sink or waste container.
  - c. Gently blot the inverted washer/plate assembly onto several layers of paper towels or absorbent surface to remove any residual liquid.
  - d. Add 150  $\mu$ L of 1X Wash Buffer into each well and wait 30 seconds.
  - e. Remove the liquid by quickly inverting the washer/plate assembly over a sink or waste container.
  - f. Gently blot the inverted washer/plate assembly onto several layers of paper towels or absorbent surface to remove any residual liquid.
  - g. Remove the plate from the magnet and proceed to step 3.
3. Add samples and Control Plasma to the plate.
    - a. **Plasma:** Add 25  $\mu$ L of 1X UAB to each well followed by 25  $\mu$ L of prepared and diluted Control Plasma or prediluted samples as defined on the plate layout. Add an additional 25  $\mu$ L of 1X UAB to the wells designated as backgrounds.
    - b. Seal the plate using one of the provided Plate Seals and cover with the provided Microplate Lid. Shake at 600 rpm for 2 hours at room temperature.
  4. Remove and discard the Plate Seal. Wash the plate following the steps below.
    - a. Place the plate on the Hand-Held Magnetic Plate Washer and wait 2 minutes to allow particles to settle on the bottom of each well.
    - b. Remove the liquid by quickly inverting the washer/plate assembly over a sink or waste container.

- c. Gently blot the inverted washer/plate assembly onto several layers of paper towels or absorbent surface to remove any residual liquid.
  - d. Add 150  $\mu$ L of 1X Wash Buffer into each well and wait 30 seconds.
  - e. Remove the liquid by quickly inverting the washer/plate assembly over a sink or waste container.
  - f. Gently blot the inverted washer/plate assembly onto several layers of paper towels or absorbent surface to remove any residual liquid.
  - g. Repeat steps 4d-4f once more for a total of two washes.
  - h. Remove the plate from the magnet and proceed to the next step.
5. Add Biotinylated detection Antibody Mix to the plate.
  - a. Using a multichannel pipette, add 25  $\mu$ L of the detection antibody solution to each well of the plate. Gently tap the plate to evenly distribute the solution in the wells.

---

**Note:** A narrow trough reservoir for multichannel pipetting is recommended to be used to prevent volume loss.

---
- b. Seal the plate using a new Plate Seal and cover with the provided Microplate Lid. Shake at 600 rpm for 30 minutes at room temperature.
6. Wash the plate following step 4.
7. Add Streptavidin-PE (SA-PE) to the plate.
  - a. Add 50  $\mu$ L of SA-PE solution to each well.
  - b. Seal the plate using new Plate Seal and cover with the provided Microplate Lid. Shake at 600 rpm for 30 minutes at room temperature.
8. Wash the plate following step 4.
9. Prepare the plate for analysis on a xMAP™ instrument.
  - a. Add 120  $\mu$ L of reading buffer into each well.
  - b. Seal the plate using new Plate Seal and cover with the provided Microplate Lid. Shake at 600 rpm for 5 minutes at room temperature.
10. Remove the Plate Seal and run the plate on a xMAP™ instrument.

## Instrument settings

Follow the recommended guidelines and procedures for calibration and verification of the instrument. Laser-based systems require 30 minutes to warm up prior to use.

Instrument	Acquisition volume	Timeout (optional)	Bead type	DD gate	Reporter gain	Min. bead count
MAGPIX™	50 µL <sup>[1]</sup>	N/A	N/A	N/A	Standard PMT	50
INTELLIFLEX™	30 µL	40 sec	MagPlex™	4,000–13,000	Standard PMT	50
FLEXMAP 3D™ Luminex™ 100/200™	50 µL	60 sec	MagPlex™	7,500–25,000	Standard PMT	50
Bio-Rad™ Bio-Plex™	50 µL	60 sec	MagPlex™	5,000–25,000	Standard PMT	50

<sup>[1]</sup> MAGPIX volume can be changed during the run to optimize bead count.

---

**Note:** To assure a good bead count, the probe height must be adjusted to the plate provided in the kit. We recommend using two 5.08 mm spacer disks to adjust the sample probe height for Mylar-bottom plates.

---

## Analyze results

The concentration of the samples can be calculated by plotting the expected concentration of the Control Plasma against the NET MFI generated by the Control Plasma. For Bio-Plex™ Manager, plot Control Plasma concentrations against FI-Bkgd. A 4PL or 5PL algorithm is recommended for the best curve fit. Analyze the assayed samples according to the operation manual for the Luminex™ or Bio-Plex™ instrument.

We offer the free and robust ProcartaPlex Analyst 1.0 analysis software package for data analysis.

---

**Note:** The samples have been diluted 1:500, which must be accounted for in the software analysis.

---

**IMPORTANT!** For ProcartaPlex™ getting started guides, technical literature, protocol support tools, and common troubleshooting questions visit [thermofisher.com/procartaplexsupport](http://thermofisher.com/procartaplexsupport)  
For more complete troubleshooting questions and answers, visit our FAQ database at [thermofisher.com/procartaplexfaqs](http://thermofisher.com/procartaplexfaqs)

---



# Recommended plate layout

Control Plasma		Samples									
1	1	1	1	9	9	17	17	25	25	33	33
2	2	2	2	10	10	18	18	26	26	34	34
3	3	3	3	11	11	19	19	27	27	35	35
4	4	4	4	12	12	20	20	28	28	36	36
5	5	5	5	13	13	21	21	29	29	37	37
6	6	6	6	14	14	22	22	30	30	38	38
7	7	7	7	15	15	23	23	31	31	39	39
Bkgd <sup>[1]</sup>	Bkgd	8	8	16	16	24	24	32	32	40	40

<sup>[1]</sup> Background

	1	2	3	4	5	6	7	8	9	10	11	12
A												
B												
C												
D												
E												
F												
G												
H												



