

Human HSP27 ELISA Kit

Enzyme-linked Immunosorbent Assay for quantitative detection of human HSP27

Catalog Numbers BMS2086 or BMS2086TEN

Pub. No. MAN0016531 **Rev.** A.0 (30)

WARNING! Read the Safety Data Sheets (SDSs) and follow the handling instructions. Wear appropriate protective eyewear, clothing, and gloves. Safety Data Sheets (SDSs) are available from thermofisher.com/support.

Product description

The Human HSP27 ELISA Kit is an enzyme-linked immunosorbent assay for the quantitative detection of human HSP27.

Summary

Heat shock protein 27 (HSP27) is a member of the heat shock protein family, a group of proteins that are induced in response to stressors such as changing temperatures, cytokine levels, and presence of various chemicals. Heat shock proteins serve as molecular chaperones, binding to other proteins to maintain proper protein structure or by folding denatured proteins and preventing activation of caspases that could lead to apoptosis. Unlike the larger HSP proteins, HSP27 belongs to a unique subgroup that is involved in apoptosis regulation. Expression of HSP27 is constitutive, but upon stress HSP27 is upregulated and can relocate from the cytoplasm to the nucleus. For literature update refer to our website.

Principles of the test

An anti-human HSP27 coating antibody is adsorbed onto microwells.

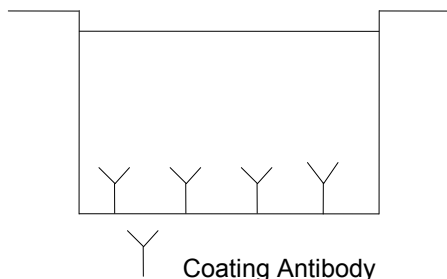


Fig. 1 Coated microwell

Human HSP27 present in the sample or standard binds to antibodies adsorbed to the microwells and a biotin-conjugated anti-human HSP27 antibody is added and binds to human HSP27 captured by the first antibody.

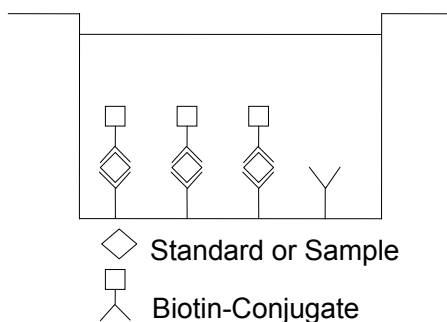


Fig. 2 First incubation

Following incubation unbound biotin-conjugated anti-human HSP27 antibody is removed during a wash step Streptavidin-HRP is added and binds to the biotin-conjugated anti-human HSP27 antibody.

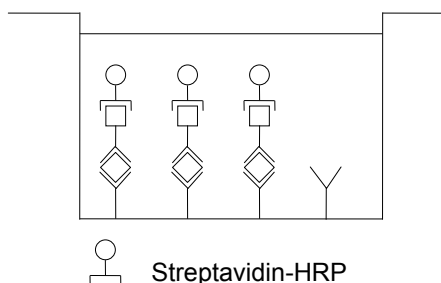


Fig. 3 Second incubation

Following incubation unbound Streptavidin-HRP is removed during a wash step, and substrate solution reactive with HRP is added to the wells.

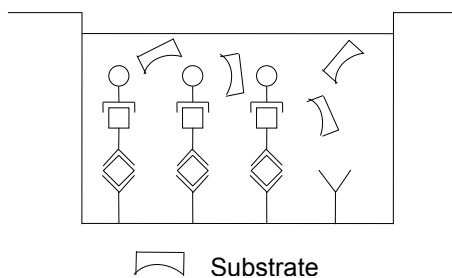


Fig. 4 Third incubation

A colored product is formed in proportion to the amount of human HSP27 present in the sample or standard. The reaction is terminated by addition of acid and absorbance is measured at 450 nm. A standard curve is prepared from 7 human HSP27 standard dilutions and human HSP27 sample concentration determined.

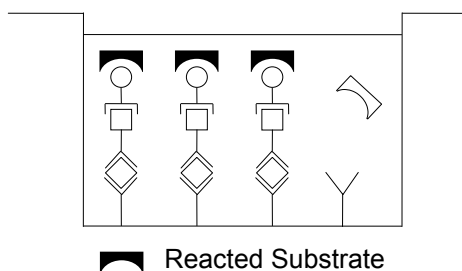


Fig. 5 Fourth incubation

Reagents provided

Reagents for human HSP27 ELISA BMS2086 (96 tests)

1 aluminum pouch with a Microwell Plate (12 strips with 8 wells each) coated with monoclonal antibody to human HSP27

1 vial (70 µL) Biotin-Conjugate anti-human HSP27 monoclonal antibody

1 vial (150 µL) Streptavidin-HRP

2 vials human HSP27 Standard lyophilized, 2000 pg/mL upon reconstitution

Note: In some, very rare cases, an insoluble precipitate of stabilizing protein has been seen in the vial. This precipitate does not interfere in any way with the performance of the test and can thus be ignored.

1 bottle (12 mL) Sample Diluent

1 vial (5 mL) Assay Buffer Concentrate 20x (PBS with 1% Tween™ 20, 10% BSA)

1 bottle (50 mL) Wash Buffer Concentrate 20x (PBS with 1% Tween™ 20)

1 vial (15 mL) Substrate Solution (tetramethyl-benzidine)

1 vial (15 mL) Stop Solution (1M Phosphoric acid)

4 Adhesive Films

Reagents for human HSP27 ELISA BMS2086TEN (10x96 tests)

10 aluminum pouches with a Microwell Plate (12 strips with 8 wells each) coated with monoclonal antibody to human HSP27

10 vials (70 µL) Biotin-Conjugate anti-human HSP27 monoclonal antibody

10 vials (150 µL) Streptavidin-HRP

10 vials human HSP27 Standard lyophilized, 2000 pg/mL upon reconstitution

Note: In some, very rare cases, an insoluble precipitate of stabilizing protein has been seen in the vial. This precipitate does not interfere in any way with the performance of the test and can thus be ignored.

10 bottles (12 mL) Sample Diluent

2 vials (5 mL) Assay Buffer Concentrate 20x (PBS with 1% Tween™ 20, 10% BSA)

5 bottles (50 mL) Wash Buffer Concentrate 20x (PBS with 1% Tween™ 20)

10 vials (15 mL) Substrate Solution (tetramethyl-benzidine)

1 vial (100 mL) Stop Solution (1M Phosphoric acid)

20 Adhesive Films

Storage instructions – ELISA kit

Store kit reagents between 2°C and 8°C. Immediately after use remaining reagents should be returned to cold storage (2°C to 8°C). Expiry of the kit and reagents is stated on labels.

Expiry of the kit components can only be guaranteed if the components are stored properly, and if, in case of repeated use of one component, this reagent is not contaminated by the first handling.

Sample collection and storage instructions

Cell lysates, cell culture supernatant, serum, and plasma (citrate, heparin, EDTA) were tested with this assay. Other biological samples might be suitable for use in the assay.

Pay attention to a possible *Hook Effect* due to high sample concentrations

Samples containing a visible precipitate must be clarified prior to use in the assay. Do not use grossly hemolyzed or lipemic specimens.

Samples should be aliquoted and must be stored frozen at –20°C to avoid loss of bioactive human HSP27.

Avoid repeated freeze-thaw cycles. Prior to assay, the frozen sample should be brought to room temperature slowly and mixed gently.

Materials required but not provided

- 5 mL and 10 mL graduated pipettes
- 5 µL to 1000 µL adjustable single channel micropipettes with disposable tips
- 50 µL to 300 µL adjustable multichannel micropipette with disposable tips
- Multichannel micropipette reservoir
- Beakers, flasks, cylinders necessary for preparation of reagents
- Device for delivery of wash solution (multichannel wash bottle or automatic wash system)
- Microplate shaker
- Microwell strip reader capable of reading at 450 nm (620 nm as optional reference wave length)
- Glass-distilled or deionized water
- Statistical calculator with program to perform regression analysis

Precautions for use

- All reagents should be considered as potentially hazardous. We therefore recommend that this product is handled only by those persons who have been trained in laboratory techniques and that it is used in accordance with the principles of good laboratory practice. Wear suitable protective clothing such as laboratory overalls, safety glasses and gloves. Care should be taken to avoid contact with skin or eyes. In the case of contact with skin or eyes wash immediately with water. See material safety data sheet(s) and/or safety statement(s) for specific advice.
- Reagents are intended for research use only and are not for use in diagnostic or therapeutic procedures.
- Do not mix or substitute reagents with those from other lots or other sources.
- Do not use kit reagents beyond expiration date on label.
- Do not expose kit reagents to strong light during storage or incubation.
- Do not pipet by mouth.
- Do not eat or smoke in areas where kit reagents or samples are handled.
- Avoid contact of skin or mucous membranes with kit reagents or samples.
- Rubber or disposable latex gloves should be worn while handling kit reagents or samples.
- Avoid contact of substrate solution with oxidizing agents and metal.
- Avoid splashing or generation of aerosols.
- To avoid microbial contamination or cross-contamination of reagents or samples that may invalidate the test, use disposable pipette tips and/or pipettes.
- Use clean, dedicated reagent trays for dispensing the conjugate and substrate reagent.
- Exposure to acid inactivates the conjugate.
- Glass-distilled water or deionized water must be used for reagent preparation.
- Substrate solution must be at room temperature prior to use.
- Decontaminate and dispose samples and all potentially contaminated materials as if they could contain infectious agents. The preferred method of decontamination is autoclaving for a minimum of 1 hour at 121.5°C.
- Liquid wastes not containing acid and neutralized waste may be mixed with sodium hypochlorite in volumes such that the final mixture contains 1.0% sodium hypochlorite. Allow 30 minutes for effective decontamination. Liquid waste containing acid must be neutralized prior to the addition of sodium hypochlorite.

Preparation of reagents

1. Buffer Concentrates should be brought to room temperature and should be diluted before starting the test procedure.
2. If crystals have formed in the Buffer Concentrates, warm them gently until they have completely dissolved.

Wash buffer (1x)

1. Pour entire contents (50 mL) of the Wash Buffer Concentrate (20x) into a clean 1000 mL graduated cylinder. Bring to final volume of 1000 mL with glass-distilled or deionized water. Mix gently to avoid foaming.
2. Transfer to a clean wash bottle and store at 2° to 25°C. Please note that Wash Buffer (1x) is stable for 30 days.
3. Wash Buffer (1x) may also be prepared as needed according to the following table:

Number of Strips	Wash Buffer Concentrate (20x) (mL)	Distilled Water (mL)
1 - 6	25	475
1 - 12	50	950

Assay buffer (1x)

1. Pour the entire contents (5 mL) of the Assay Buffer Concentrate (20x) into a clean 100 mL graduated cylinder. Bring to final volume of 100 mL with distilled water. Mix gently to avoid foaming.
2. Store at 2° to 8°C. Please note that the Assay Buffer (1x) is stable for 30 days.
3. Assay Buffer (1x) may also be prepared as needed according to the following table:

Number of Strips	Assay Buffer Concentrate (20x) (mL)	Distilled Water (mL)
1 - 6	2.5	47.5
1 - 12	5.0	95.0

Biotin-Conjugate

Note: The Biotin-Conjugate should be used within 30 minutes after dilution.

Make a 1:100 dilution of the concentrated Biotin-Conjugate solution with Assay Buffer (1x) in a clean plastic tube as needed according to the following table:

Number of Strips	Biotin-Conjugate (mL)	Assay Buffer (1x) (mL)
1 - 6	0.03	2.97
1 - 12	0.06	5.94

Streptavidin-HRP

Note: The Streptavidin-HRP should be used within 30 minutes after dilution.

Make a 1:100 dilution of the concentrated Streptavidin-HRP solution with Assay Buffer (1x) in a clean plastic tube as needed according to the following table:

Number of Strips	Streptavidin-HRP (mL)	Assay Buffer (1x) (mL)
1 - 6	0.06	5.94
1 - 12	0.12	11.88

Human HSP27 standard

1. Reconstitute human HSP27 standard by addition of distilled water. Reconstitution volume is stated on the label of the standard vial. Swirl or mix gently to insure complete and homogeneous solubilization (concentration of reconstituted standard = 2000 pg/mL).
2. Allow the standard to reconstitute for 10-30 minutes. Mix well prior to making dilutions.
3. The standard has to be used immediately after reconstitution and cannot be stored.
4. Standard dilutions can be prepared directly on the microwell plate (see "Test protocol" on page 3) or alternatively in tubes (see "External standard dilution" on page 3).

External standard dilution

1. Label 7 tubes, one for each standard point: S1, S2, S3, S4, S5, S6, S7.
2. Prepare 2-fold serial dilutions for the standard curve as follows: Pipette 225 µL of Sample Diluent into each tube.
3. Pipette 225 µL of reconstituted standard (concentration = 2000 pg/mL) into the first tube, labeled S1, and mix (concentration of S1 = 1000 pg/mL).
4. Pipette 225 µL of this dilution into the second tube, labeled S2, and mix thoroughly before the next transfer.
5. Repeat serial dilutions 5 more times thus creating the points of the standard curve (see Figure 6).

Sample Diluent serves as blank.

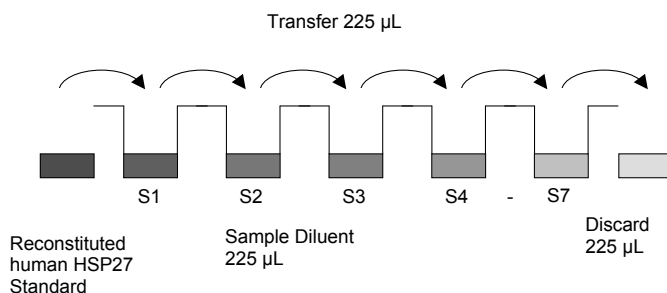


Fig. 6 Dilute standards - tubes

Test protocol

If instructions of this protocol have been followed samples have been diluted 1:10, the concentration read from the standard curve must be multiplied by the dilution factor (x 10).

Shaking is absolutely necessary for an optimal test performance.

1. Determine the number of microwell strips required to test the desired number of samples plus appropriate number of wells needed for running blanks and standards. Each sample, standard, blank and optional control sample should be assayed in duplicate. Remove extra microwell strips from holder and store in foil bag with the desiccant provided at 2–8°C sealed tightly.
2. Prepare Biotin-Conjugate (see "Biotin-Conjugate" on page 3).
3. Wash the microwell strips twice with approximately 400 µL Wash Buffer per well with thorough aspiration of microwell contents between washes. Allow the Wash Buffer to sit in the wells for about 10–15 seconds before aspiration. Take care not to scratch the surface of the microwells.

After the last wash step, empty wells and tap microwell strips on absorbent pad or paper towel to remove excess Wash Buffer. Use the microwell strips immediately after washing. Alternatively microwell strips can be placed upside down on a wet absorbent paper for not longer than 15 minutes. Do not allow wells to dry.

4. Standard dilution on the microwell plate (alternatively, the standard dilution can be prepared in tubes, see "External standard dilution" on page 3):

Add 100 µL of Sample Diluent in duplicate to all standard wells. Pipette 100 µL of prepared standard (see "Human HSP27 standard" on page 3, concentration = 2,000 pg/mL), in duplicate, into well A1 and A2 (see Table 1). Mix the contents of wells A1 and A2 by repeated aspiration and ejection (concentration of standard 1 S1 = 1,000 pg/mL), and transfer 100 µL to wells B1 and B2, respectively (see Figure 7). Take care not to scratch the inner surface of the microwells. Continue this procedure 5 times, creating two rows of human HSP27 standard dilutions, ranging from 1,000 pg/mL to 15.6 pg/mL. Discard 100 µL of the contents from the last microwells (S7) used.

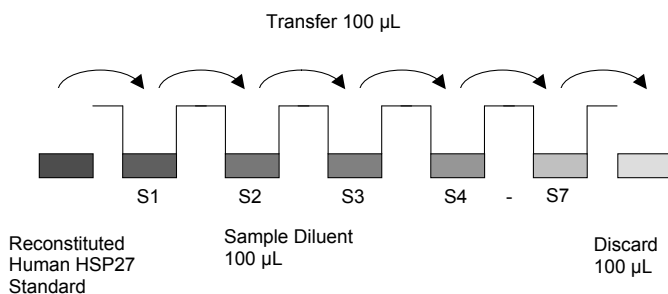


Fig. 7 Dilute standards - microwell plate.

In case of an external standard dilution (see “External standard dilution” on page 3), pipette 100 µL of these standard dilutions (S1–S7) in the standard wells according to Table 1.

Table 1 Example of the arrangement of blanks, standards, and samples in the microwell strips.

	1	2	3	4
A	Standard 1 1,000 pg/mL	Standard 1 1,000 pg/mL	Sample 1	Sample 1
B	Standard 2 500 pg/mL	Standard 2 500 pg/mL	Sample 2	Sample 2
C	Standard 3 250 pg/mL	Standard 3 250 pg/mL	Sample 3	Sample 3
D	Standard 4 125 pg/mL	Standard 4 125 pg/mL	Sample 4	Sample 4
E	Standard 5 62.5 pg/mL	Standard 5 62.5 pg/mL	Sample 5	Sample 5
F	Standard 6 31.3 pg/mL	Standard 6 31.3 pg/mL	Sample 6	Sample 6
G	Standard 7 15.6 pg/mL	Standard 7 15.6 pg/mL	Sample 7	Sample 7
H	Blank	Blank	Sample 8	Sample 8

- Add 100 µL of Sample Diluent in duplicate to the blank wells.
- Add 90 µL of Sample Diluent to the sample wells.
- Add 10 µL of each sample in duplicate to the sample wells.
- Add 50 µL of diluted Biotin-Conjugate to all wells, including the blank wells.
- Cover with an adhesive film and incubate at room temperature (18–25°C) for 2 hours on a microplate shaker. (Shaking is absolutely necessary for an optimal test performance.)
- Prepare Streptavidin-HRP (see “Streptavidin-HRP” on page 3).
- Remove adhesive film and empty wells. Wash microwell strips 4 times according to point 2 of the test protocol. Proceed immediately to the next step.
- Add 100 µL of diluted Streptavidin-HRP to all wells, including the blank wells. Cover with an adhesive film and incubate at room temperature (18–25°C) for 1 hour on a microplate shaker. (Shaking is absolutely necessary for an optimal test performance.)
- Remove adhesive film and empty wells. Wash microwell strips 4 times according to point 2 of the test protocol. Proceed immediately to the next step.
- Pipette 100 µL of TMB Substrate Solution to all wells.
- Incubate the microwell strips at room temperature (18–25°C) for 30 minutes. Avoid direct exposure to intense light.

The color development on the plate should be monitored and the substrate reaction stopped (see next point of this protocol) before positive wells are no longer properly recordable. Determination of the ideal time period for color development has to be done individually for each assay.

It is recommended to add the stop solution when the highest standard has developed a dark blue color. Alternatively the color development can be monitored by the ELISA reader at 620 nm. The substrate reaction should be stopped as soon as Standard 1 has reached an OD of 0.9–0.95.

- Stop the enzyme reaction by quickly pipetting 100 µL of Stop Solution into each well. It is important that the Stop Solution is spread quickly and uniformly throughout the microwells to completely inactivate the enzyme. Results must be read immediately after the Stop Solution is added or within one hour if the microwell strips are stored at 2–8°C in the dark.
- Read absorbance of each microwell on a spectro-photometer using 450 nm as the primary wave length (optionally 620 nm as the reference wave length; 610 nm to 650 nm is acceptable). Blank the plate reader according to the manufacturer's instructions by using the blank wells. Determine the absorbance of both the samples and the standards.

Calculation of results

- Calculate the average absorbance values for each set of duplicate standards and samples. Duplicates should be within 20 percent of the mean value.
- Create a standard curve by plotting the mean absorbance for each standard concentration on the ordinate against the human HSP27 concentration on the abscissa. Draw a best fit curve through the points of the graph (a 5-parameter curve fit is recommended).
- To determine the concentration of circulating human HSP27 for each sample, first find the mean absorbance value on the ordinate and extend a horizontal line to the standard curve. At the point of intersection, extend a vertical line to the abscissa and read the corresponding human HSP27 concentration.
- If instructions in this protocol have been followed, samples have been diluted 1:10 (10 µL sample + 90 µL Sample Diluent) and the concentration read from the standard curve must be multiplied by the dilution factor (x 10).
- Calculation of samples with a concentration exceeding standard 1 may result in incorrect, low human HSP27 levels (Hook Effect). Such samples require further external predilution according to expected human HSP27 values with Sample Diluent in order to precisely quantitate the actual human HSP27 level.
- It is suggested that each testing facility establishes a control sample of known human HSP27 concentration and runs this additional control with each assay. If the values obtained are not within the expected range of the control, the assay results may be invalid.

- A representative standard curve is shown in Figure 8.
Note: Do not use this standard curve to derive test results. Each laboratory must prepare a standard curve for each group of microwell strips assayed.

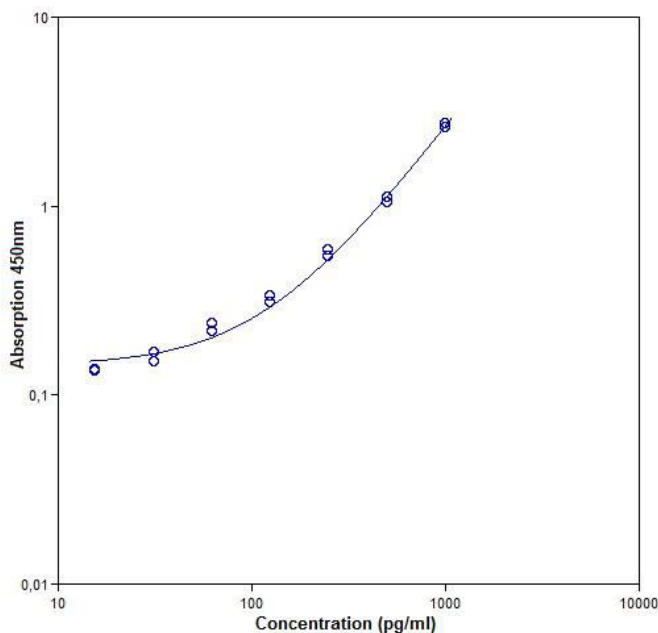


Fig. 8 Representative standard curve for human HSP27 ELISA. Human HSP27 was diluted in serial 2-fold steps in Sample Diluent.

Table 2 Typical data using the human HSP27 ELISA.

Measuring wavelength: 450 nm

Reference wavelength: 620 nm

Standard	human HSP27 Concentration (pg/mL)	O.D. at 450 nm	Mean O.D. at 450 nm	C.V. (%)
1	1000	2.614 2.735	2.674	2.3
2	500	1.052 1.112	1.082	2.8
3	250	0.543 0.590	0.567	4.2
4	125	0.310 0.333	0.321	3.5
5	62.5	0.238 0.218	0.228	4.5
6	31.3	0.169 0.151	0.160	5.8
7	15.6	0.136 0.134	0.135	0.6
Blank	0.0	0.119 0.100	0.110	

The OD values of the standard curve may vary according to the conditions of assay performance (e.g., operator, pipetting technique, washing technique, or temperature effects). Furthermore, shelf life of the kit may affect enzymatic activity and thus color intensity. Values measured are still valid.

Limitations

- Since exact conditions may vary from assay to assay, a standard curve must be established for every run.
- Bacterial or fungal contamination of either screen samples or reagents or cross-contamination between reagents may cause erroneous results.

- Disposable pipette tips, flasks or glassware are preferred, reusable glassware must be washed and thoroughly rinsed of all detergents before use.
- Improper or insufficient washing at any stage of the procedure will result in either false positive or false negative results. Empty wells completely before dispensing fresh wash solution, fill with Wash Buffer as indicated for each wash cycle and do not allow wells to sit uncovered or dry for extended periods.

Performance characteristics

Sensitivity

The limit of detection of human HSP27 defined as the analyte concentration resulting in an absorbance significantly higher than that of the dilution medium (mean plus 2 standard deviations) was determined to be 10.9 pg/mL (mean of 4 independent assays).

Reproducibility

Intra-assay

Reproducibility within the assay was evaluated in 3 independent experiments. Each assay was carried out with 6 replicates of 8 serum, plasma, cell culture supernatant samples containing different concentrations of human HSP27. Two standard curves were run on each plate. Data below show the mean human HSP27 concentration and the coefficient of variation for each sample (see Table 3). The calculated overall intra-assay coefficient of variation was 5.8%.

Table 3 The mean human HSP27 concentration and the coefficient of variation for each sample.

Sample	Experiment	Mean human HSP27 concentration (pg/mL)	Coefficient of variation (%)
1	1	9,425.5	2.9
	2	9,945.6	2.6
	3	9,568.4	2.3
2	1	4,879.8	2.7
	2	5,276.3	1.4
	3	4,936.4	2.0
3	1	803.6	8.1
	2	870.3	5.7
	3	847.8	7.3
4	1	418.0	13.1
	2	511.0	3.5
	3	465.3	5.6
5	1	1,814.7	2.3
	2	1,870.7	7.8
	3	1,818.1	2.0
6	1	1,375.5	9.4
	2	1,426.0	11.6
	3	1,471.6	5.6
7	1	2,825.8	4.8
	2	2,825.1	10.4
	3	2,688.7	6.9
8	1	1,669.4	4.5
	2	1,506.2	14.6
	3	1,575.3	1.7

Inter-assay

Assay to assay reproducibility within one laboratory was evaluated in 3 independent experiments. Each assay was carried out with 6 replicates of 8 serum, plasma, cell culture supernatant samples containing different concentrations of human HSP27. Two standard curves were run on each plate. Data below show the mean human HSP27 concentration and the coefficient of variation calculated on

18 determinations of each sample (see Table 4). The calculated overall inter-assay coefficient of variation was 4.3%.

Table 4 The mean human HSP27 concentration and the coefficient of variation of each sample.

Sample	Mean human HSP27 concentration (pg/mL)	Coefficient of variation (%)
1	9,646.5	2.8 %
2	5,030.9	4.3 %
3	840.6	4.0 %
4	464.8	10.0 %
5	1,834.5	1.7 %
6	1,424.4	3.4 %
7	2,779.9	2.8 %
8	1,583.6	6.9 %

Spike recovery

The spike recovery was evaluated by spiking 3 levels of human HSP27 into serum, plasma (EDTA, heparin, citrate), and cell culture supernatant. Recoveries were determined with 2 replicates each. The amount of endogenous human HSP27 in unspiked samples was subtracted from the spike values.

Sample matrix	Spike high (%)		Spike medium (%)		Spike low (%)	
	Mean	Range	Mean	Range	Mean	Range
Serum	91	84–96	94	88–99	99	90–106
Plasma (EDTA)	95	78–114	86	65–99	94	72–122
Plasma (citrate)	93	90–98	90	83–94	89	79–107
Plasma (heparin)	75	69–78	80	74–83	79	74–85
Cell culture supernatant	97	95–99	106	103–109	86	85–87

Dilution parallelism

Serum, plasma (EDTA, citrate, heparin), and cell culture supernatant samples with different levels of human HSP27 were analyzed at serial 2-fold dilutions with 4 replicates each.

Sample matrix	Dilution	Recovery of Exp. Val. (%)	
		Mean	Range
Serum	1:20	82	74–89
	1:40	75	66–85
	1:80	82	64–96
Plasma (EDTA)	1:20	98	91–105
	1:40	99	94–109
	1:80	101	95–110
Plasma (citrate)	1:20	99	88–112
	1:40	105	96–113
	1:80	107	60–125
Plasma (heparin)	1:20	90	79–95
	1:40	84	78–96
	1:80	82	73–88
Cell culture supernatant	1:2	97	97–101
	1:4	90	90–90
	1:8	68	68–69

Sample stability

Freeze-Thaw stability

Aliquots of serum, plasma, cell culture supernatant samples (spiked or unspiked) were stored at -20°C and thawed 3 times, and the human HSP27 levels determined.

There was no significant loss of human HSP27 immunoreactivity detected by freezing and thawing.

Storage stability

Aliquots of serum, plasma, and cell culture supernatant samples (spiked or unspiked) were stored at -20°C, 2–8°C, room temperature, and at 37°C, and the human HSP27 level determined after 24 hours. There was no significant loss of human HSP27 immunoreactivity detected during storage under above conditions.

Specificity

The assay detects both natural and recombinant human HSP27. The cross-reactivity and interference of circulating factors of the immune system was evaluated by spiking these proteins at physiologically relevant concentrations into a human HSP27 positive sample. No cross-reactivity or interference was detected.

Reagent preparation summary

Wash buffer (1x)

Add Wash Buffer Concentrate 20x (50 mL) to 950 mL distilled water.

Number of Strips	Wash Buffer Concentrate (mL)	Distilled Water (mL)
1 - 6	25	475
1 - 12	50	950

Assay buffer (1x)

Add Assay Buffer Concentrate 20x (5 mL) to 95 mL distilled water.

Number of Strips	Assay Buffer Concentrate (mL)	Distilled Water (mL)
1 - 6	2.5	47.5
1 - 12	5.0	95.0

Biotin-Conjugate

Make a 1:100 dilution of the concentrated Biotin-Conjugate solution with Assay Buffer (1x) in a clean plastic tube as needed according to the following table:

Number of Strips	Biotin-Conjugate (mL)	Assay Buffer (1x) (mL)
1 - 6	0.03	2.97
1 - 12	0.06	5.94

Streptavidin-HRP

Make a 1:100 dilution of the concentrated Streptavidin-HRP solution with Assay Buffer (1x) in a clean plastic tube as needed according to the following table:

Number of Strips	Streptavidin-HRP (mL)	Assay Buffer (1x) (mL)
1 - 6	0.06	5.94
1 - 12	0.12	11.88

Human HSP27 standard

Reconstitute human HSP27 standard with distilled water. (Reconstitution volume is stated on the label of the standard vial.)

Test protocol summary

Note: If instructions of this protocol have been followed, samples have been diluted 1:10 and the concentration read from the standard curve must be multiplied by the dilution factor (x 10).

1. Determine the number of microwell strips required.
2. Prepare Biotin-Conjugate.
3. Wash microwell strips twice with Wash Buffer.
4. Standard dilution on the microwell plate: Add 100 µl Sample Diluent, in duplicate, to all standard wells. Pipette 100 µl prepared standard into the first wells and create standard dilutions by transferring 100 µl from well to well. Discard 100 µl from the last wells.

Alternatively, external standard dilution in tubes (see “External standard dilution” on page 3): Pipette 100 µl of these standard dilutions in the microwell strips.

5. Add 100 µL of Sample Diluent in duplicate to the blank wells.
6. Add 90 µL of Sample Diluent to the sample wells.
7. Add 10 µL of each sample in duplicate to the sample wells.
8. Add 50 µL diluted Biotin-Conjugate to all wells.
9. Cover microwell strips and incubate 2 hours at room temperature (18–25°C) on a microplate shaker. (Shaking is absolutely necessary for an optimal test performance.)
10. Prepare Streptavidin-HRP.
11. Empty and wash microwell strips 4 times with Wash Buffer.
12. Add 100 µL diluted Streptavidin-HRP to all wells.
13. Cover microwell strips and incubate 1 hours at room temperature (18–25°C) on a microplate shaker. (Shaking is absolutely necessary for an optimal test performance.)
14. Empty and wash microwell strips 4 times with Wash Buffer.
15. Add 100 µL of TMB Substrate Solution to all wells.
16. Incubate the microwell strips for about 30 minutes at room temperature (18–25°C)
17. Add 100 µL Stop Solution to all wells.
18. Blank microwell reader and measure color intensity at 450 nm.

- Product support information
 - Product FAQs
 - Software, patches, and updates
 - Training for many applications and instruments
- Order and web support
- Product documentation
 - User guides, manuals, and protocols
 - Certificates of Analysis
 - Safety Data Sheets (SDSs; also known as MSDSs)

Note: For SDSs for reagents and chemicals from other manufacturers, contact the manufacturer.

Limited product warranty

Life Technologies Corporation and/or its affiliate(s) warrant their products as set forth in the Life Technologies' General Terms and Conditions of Sale at www.thermofisher.com/us/en/home/global/terms-and-conditions.html. If you have any questions, please contact Life Technologies at www.thermofisher.com/support.

Customer and technical support

Visit thermofisher.com/support for the latest service and support information.

- Worldwide contact telephone numbers



Bender MedSystems GmbH | Campus Vienna Biocenter 2 | 1030 Vienna, Austria

For descriptions of symbols on product labels or product documents, go to thermofisher.com/symbols-definition.

The information in this guide is subject to change without notice.

DISCLAIMER: TO THE EXTENT ALLOWED BY LAW, THERMO FISHER SCIENTIFIC INC. AND/OR ITS AFFILIATE(S) WILL NOT BE LIABLE FOR SPECIAL, INCIDENTAL, INDIRECT, PUNITIVE, MULTIPLE, OR CONSEQUENTIAL DAMAGES IN CONNECTION WITH OR ARISING FROM THIS DOCUMENT, INCLUDING YOUR USE OF IT.

Important Licensing Information: These products may be covered by one or more Limited Use Label Licenses. By use of these products, you accept the terms and conditions of all applicable Limited Use Label Licenses.

©2018 Thermo Fisher Scientific Inc. All rights reserved. All trademarks are the property of Thermo Fisher Scientific and its subsidiaries unless otherwise specified. All other trademarks are the property of their respective owners.