

Floor 1-4, Building #8, Optics Valley Precision Medicine Industry Base Phase I, #9 Gaokeyuan 3rd Road,
East Lake High-Tech Zone, Wuhan City, Hubei Province, People's Republic of China.

For Professional Use

MYC(8q24)/BCL6(3q27)/BCL2(18q21) gene break apart probe reagent Instructions Manual

[Product Name] MYC(8q24)/BCL6(3q27)/BCL2(18q21) gene break apart probe reagent

[Package Specifications] 10 Tests/box

[Intended use]

The reagent carries out in situ hybridization staining on the basis of routine staining to provide doctors with auxiliary information for diagnosis. The test results are only for clinical reference and should not be used as the only basis for clinical diagnosis. Clinicians should comprehensively judge the test results in combination with the patient's condition, drug indications, treatment response and other laboratory test indicators.

[Detection principle]


Fluorescence in situ hybridization is a technique for directly observing specific nucleic acids in cells in vitro. According to the principle of base complementary pairing, the specific probe is complementary to the target sequence in the cell. Due to the fluorescence of the probe, the gene state of the hybrid probe and the target sequence can be clearly observed under the fluorescence microscope under the appropriate excitation light.

[Product Main Components]

The kit consists of one of MYC, BCL6 or BCL2 dual color probe as shown in Table 1.

Table 1 Kit composition

Cat#	Component name	Specifications	Quantity	Main components
FP-243-1	MYC dual color probe	100μl/Tube	1	MYC Orange probe、MYC Green probe、hybridization buffer
FP-243-2	BCL6 dual color probe	100μl/Tube	1	BCL6 Orange probe、BCL6 Green probe、hybridization buffer
FP-243-3	BCL2 dual color probe	100μl/Tube	1	BCL2 Orange probe、BCL2 Green probe、hybridization buffer

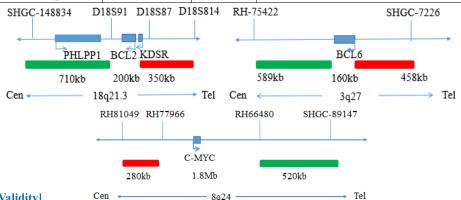

[Storage conditions & Validity]

Keep sealed away from light at -20°C±5°C. The product is valid for 12 months. Avoid unnecessary repeated freezing and thawing that should not exceed 10 times. After opening, within 24 hours for short-term preservation, keep sealed at 2-8°C in dark. For long-term preservation after opening, keep the lid sealed at -20°C±5°C away from light. The kit is transported below 0°C.

[Applicable Instruments]

Fluorescence microscopy imaging systems, including fluorescence microscopy and filter sets suitable for DAPI (367/452), Green (495/517), and Orange (547/565).

[Sample Requirements]

Tissue samples:

- 1. Applicable specimen type: paraffin embedded specimen of surgical resection or biopsy tissue.
- 2. The tissue should be fixed with 4% neutral formaldehyde fixation solution within 1 hour after in vitro. After tissue fixation, it should be regularly dehydrated and embedded in paraffin.

Cell sample:

- 1. Applicable specimen type: unfixed fresh bone marrow specimen (stored at 2-8 °C for no more than 24 hours).
- 2. Sample collection take 1-3ml of bone marrow cells anticoagulated with heparin sodium.
- 3. Sample preservation: after fixation, the cell suspension shall be stored at -20±5 °C for no more than 12 months; The prepared cell slides can be

	Wuhan HealthCare	Biotechnology (C o. ,
l td			

Wuhan HealthCare Biotechnology Co., Ltd.



Floor 1-4, Building #8, Optics Valley Precision Medicine Industry Base Phase I, #9 Gaokeyuan 3rd Road, East Lake High-Tech Zone, Wuhan City, Hubei Province, People's Republic of China.

stored at -20±5 °C for no more than 1 month. When the sample storage temperature is too high or too low, or the cell suspension is volatilized excessively or polluted during storage, the sample will not be used for detection.

[Test method]

1.Related Reagents

The following reagents are required for the experiment but not provided in this kit

(1) $20 \times SSC$, pH 5.3 ± 0.2

Weigh 176g of sodium chloride and 88g of sodium citrate, dissolve in 800mL of deionized water, adjust the pH to 5.3±0.2 at room temperature, and complete to 1 L with deionized water. High-pressure steam sterilization, stored at 2-8°C, the solution shelf life is of 6 months. Discard if the reagent appears cloudy (turbid) or contaminated.

(2) $2 \times SSC$, pH 7.0 ± 0.2

Take 100mL of the above 20xSSC, dilute with 800mL deionized water, mix, adjust the pH to 7.0±0.2 at room temperature, complete to 1L with deionized water, stored at 2-8°C, the shelf life is of 6 months. Discard if the reagent appears cloudy (turbid) or contaminated.

3 Ethanol Solution: 70% ethanol, 85% ethanol

Dilute 700ml, 850ml of ethanol with deionized water to 1L. The shelf life is of 6 months. Discard if the reagent appears cloudy (turbid) or contaminated.

4 0.3% NP-40/0.4xSSC solution, pH 7.0-7.5

Take 0.6mL NP-40 and 4mL 20×SSC, add 150mL deionized water, mix, adjust the pH to 7.0-7.5 at room temperature, with deionized water complete to a volume of 200mL. Stored at 2-8°C, the shelf life is of 6 months. Discard if the reagent appears cloudy (turbid) or contaminated.

(5) Fixation solution (methanol: glacial acetic acid = 3:1)

Prepare a ready to use fixation solution by mixing thoroughly 30ml of methanol and 10ml of glacial acetic acid.

6 0.075M KCl solution

Weigh 2.8g of potassium chloride, dissolve in 400mL of deionized water and complete to 500mL with deionized water. Stored at room temperature, the solution shelf life is of 6 months. Discard if the reagent appears cloudy (turbid) or contaminated.

(7) Diamidinyl phenylindole (DAPI) counterstain

Use commercially available anti-quenching DAPI counterstain.

2. Slides pretreatment

Tissue samples:

It is recommended to use Wuhan HealthCare Biotechnology Co., Ltd. pretreatment reagent kit.

Cell sample:

- (1) Sample collection: Take 3mL of anticoagulated bone marrow cell samples.
- (2) Cell harvesting: Place 3 mL of anticoagulated peripheral blood in a 15 mL centrifuge tube, centrifuge at 500g for 5 min, carefully discard the supernatant, and resuspend about 500µL of the residue.
- (3) Cell washing: Add 5 mL of $1 \times PBS$ buffer, mix and resuspend the cell pellet, centrifuge at 500g for 5 min, carefully discard the supernatant, and resuspend the cells with about $500\mu L$ of the residue; repeat 1 time.
- (4) Cells hypotonicty: Add 10mL of hypotonic solution pre-warmed to 37°C and place in an water bath at 37°C for 15-20min.
- (5) Cells pre-fixation: Pre-fix the cells by adding 1mL (10% by volume) of fixative solution to the cell suspension after the completion of hypotonic osmosis. Gently pipette, mix and centrifuge for 5 min at 500g, discard the supernatant, and resuspend about 500 µL of the residue.
- (6) Cell fixation: Slowly add 10mL of fixative solution to the cell suspension at room temperature for 10 min, centrifuge at 500g for 5 min, and resuspend the cells with about 500μL of the residue; repeat once (the cells may be fixed several times until the cells pellet is washed and cleaned).
- (7) Cell suspension preparation: Pipet the supernatant and add the appropriate amount of fixative solution to prepare the appropriate cell suspension concentration.
- (8) Slides preparation: Pipet 3-5µl of cell suspension drop onto the slides, put at 56°C for 30min.
- (9) Pretreatment: At room temperature, rinse the glass slides twice with 2xSSC (pH 7.0) solution for 5min each time...
- (10) Dehydration: Place the glass slides in 70% ethanol, 85% ethanol and 100% ethanol and dry for 2 minutes.

3. Denaturation and Hybridization

The following operations should be performed in a darkroom.

Tissue samples:

	_Wuhan HealthCare Biotechnolog	y Co.
Itd.		

Wuhan HealthCare Biotechnology Co., Ltd.



Floor 1-4, Building #8, Optics Valley Precision Medicine Industry Base Phase I, #9 Gaokeyuan 3rd Road, East Lake High-Tech Zone, Wuhan City, Hubei Province, People's Republic of China.

- (1) Take out the probe put at room temperature for 5min. Mix and centrifuge briefly. Take 10µl droplet in the cell and drop in the hybridization zone, immediately cover 22mmx22mm glass slide area; spread evenly without bubbles the probe under the glass slide covered area and seal edges with rubber (edge sealing must be thorough to prevent dry film from affecting the test results during hybridization).
- 2 Place the glass slides in the hybridization instrument, denature at 85°C for 5 minutes (the hybridizer should be preheated to 85°C) and hybridize at 42°C for 2 to 16 hours.

Cell sample:

- (1) Take out the probe put at room temperature for 5min. Mix and centrifuge briefly. Take 10µl droplet in the cell and drop in the hybridization zone, immediately cover 22mmx22mm glass slide area; spread evenly without bubbles the probe under the glass slide covered area and seal edges with rubber (edge sealing must be thorough to prevent dry film from affecting the test results during hybridization).
- 2 Place the glass slides in the hybridization instrument, denature at 88°C for 2 minutes (the hybridizer should be preheated to 88°C) and hybridize at 45°C for 2 to 16 hours.

4. Washing

The following operations should be performed in a darkroom.

- 1 Take out the hybridized glass slides, remove the rubber on the coverslip and immediately immerse the slides in a 2xSSC solution for 5 seconds and remove the coverslip.
- 2 Place the slides in a 2×SSC at room temperature for 1 min.
- (3) Take out the slides and immerse in a preheated at 68°C 0.3% NP-40/0.4xSSC solution and wash for 2min.
- (4) Remove the slides and immerse in a 37°C preheated deionized water, wash for 1 min and dry the slides naturally in the dark.

5. Counterstaining

The following operations should be performed in a darkroom

10µl DAPI compound dye is dropped in the hybridization area of the glass slide and immediately covered. The suitable filter is selected for glass slide observation under the fluorescence microscope.

6. FISH results observation

Put the counterstained cell drops under the fluorescence microscope, first under the low-power objective lens ($10 \times$) Confirm the cell area under the microscope; Go to $40 \times$ Under the objective lens, find a position where the cells are evenly distributed; Then in the high-power objective (100×10^{-5}) Confirm the cell area under the microscope; Go to 40×10^{-5}) Confirm the microscope the microscope

×) The FISH results of nuclei were observed.

[Common Signal Type Interpretation]

• MYC		• BCL6		• BCL2	
• MYC		• BCL6		• BCL2	
	Negative : 2 Fusion		Negative : 2 Fusion		Negative : 2 Fusion
	Positive: 1 Orange 1 Green 1 Fusion		Positive: 1 Orange 1 Green 1 Fusion		Positive: 1 Orange 1 Green 1 Fusion

[Limitations of test methods]

- 1 The results of this kit will be affected by various factors of the sample itself, but also limited by hybridization temperature and time, operating environment and the limitations of current molecular biology technology, which may lead to wrong results.
- (2) Users must understand the potential errors and accuracy limitations that may exist in the detection process.

[Precautions]

- 1. This product is only used for in vitro diagnosis.
- 2. Please read this manual carefully before testing. The testing personnel shall receive professional technical training, and the signal counting personnel must be able to observe and distinguish orange and green signals.
- 3. When testing clinical samples, when the hybridization signal counting is difficult and the sample is not enough to repeat the retest, or the cell volume is not enough for analysis, the test will not provide test results.
- 4. DAPI counterstaining agent used in this experiment has potential toxicity or carcinogenicity, so it is necessary to operate in the fume hood, wear masks and gloves to avoid direct contact.

	Wuhan HealthCare Biotechnology	Co.
l td		





Floor 1-4, Building #8, Optics Valley Precision Medicine Industry Base Phase I, #9 Gaokeyuan 3rd Road, East Lake High-Tech Zone, Wuhan City, Hubei Province, People's Republic of China.

5. All chemicals are potentially dangerous. Avoid direct contact. Used kits are clinical waste and should be properly disposed of.

[Basic information]

Name of registrant / manufacturer: Wuhan HealthCare Biotechnology Co., Ltd.

Address: Floor 1-4, Building #8, Optics Valley Precision Medicine Industry Base Phase I, #9 Gaokeyuan 3rd Road, East Lake High-Tech Zone,

Wuhan City, Hubei Province, People's Republic of China.

Contact: 027-87570662

Name of after-sales service unit: Wuhan HealthCare Biotechnology Co., Ltd.

Contact: 18140559890

Production address: Floor 1-4, Building #8, Optics Valley Precision Medicine Industry Base Phase I, #9 Gaokeyuan 3rd Road, East Lake

High-Tech Zone, Wuhan City, Hubei Province, People's Republic of China.

[medical device registration certificate No. / product technical requirement No.]

Medical device registration certificate No.: ehxb20190942 [approval date and modification date of the specification]

V1. 0 approval date: October 29, 2019 V1. 2 approval date: December 7, 2021

Manufacturer

Wuhan HealthCare Biotechnology Co., Ltd.

Floor 1-4, Building #8, Optics Valley Precision Medicine Industry Base Phase I, #9 Gaokeyuan 3rd Road, East Lake High-Tech Zone, Wuhan City, Hubei Province, People's Republic of China.

E-mail: cs@healthcare-bio.com; Website: www.healthcare-biotech.com

European Representative

Kingsmead Service B.V.

Zonnehof 36, 2632 BE, Nootdorp, Netherland

 Wuhan	HealthCare	Biotechnology	Co.