Floor 1-4, Building #8, Optics Valley Precision Medicine Industry Base Phase I, #9 Gaokeyuan 3rd Road,
East Lake High-Tech Zone, Wuhan City, Hubei Province, People's Republic of China.

For Professional Use

BCL6/IGH gene fusion t(3;14) probe reagent Instructions Manual

[Product Name] BCL6/IGH gene fusion t(3;14) probe reagent

[Package Specifications] 10 Tests/box

[Intended Usage]

This kit performs fluorescence in situ hybridization staining based on conventional staining, and provides auxiliary information for diagnosis for physicians. The test results are for clinical reference only and should not be used as the sole basis for clinical diagnosis. Clinicians should make comprehensive judgments on the test results based on factors such as the patient's condition, drug indications, treatment response and other laboratory test indicators.


[Detection Principle]

Fluorescence in situ hybridization is a technique for directly observing specific nucleic acids in cells in vitro. According to the principle of complementary base pairing, a specific probe binds complementary to the target sequence in the cell. Since the probe carries fluorescein, the hybridization probe and target sequence can be clearly observed under the fluorescence microscope under the appropriate excitation light.

[Product Main Components]

This kit consists of BCL6/IGH dual-color probes, as shown in Table 1.

Table 1 Kit composition

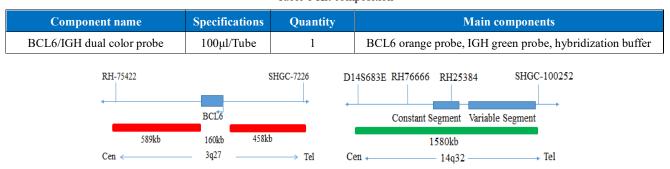

[Storage conditions & Validity]

Keep sealed away from light at -20°C±5°C, and the validity period is 12 months.

After the cover is opened, it can be sealed and stored in $2\sim8$ °C away from light within 24 hours. After the cover is opened, it should be sealed and stored in -20 ± 5 °C away from light for a long time. Transport with temperature below 0°C.

[Applicable Instruments]

Fluorescence microscopy imaging systems, including fluorescence microscopy and filter sets suitable for DAPI (367/452), Green (495/517), and Orange (547/565).

[Sample Requirements]

Cell:

- 1. Take 1-3ml of heparin sodium anticoagulant bone marrow cells.
- 2. Sample preservation: Fresh bone marrow specimen without fixation (preserved at 2-8°C for no more than 24 hours). After fixation, the cell suspension can be preserved at -20±5°C for no more than 12 months; the prepared cell slide can be preserved at -20±5°C for no more than 1 month. When the storage temperature of the sample is too high or too low, the cell suspension is volatilized excessively or polluted, the sample cannot be used for detection.

Tissue:

- 1. Applicable specimen types: Paraffin-embedded specimens from surgical excision or biopsy.
- 2. The tissue should be fixed with 4% neutral formaldehyde solution within 1 hour after isolation. After tissue fixation, it is routinely dehydrated and embedded in paraffin.

[Tests method]

1.Related reagents

(1) $20 \times SSC$, pH 5.3±0.2

Wuhan HealthCare Biotechnology Co., Ltd.



Floor 1-4, Building #8, Optics Valley Precision Medicine Industry Base Phase I, #9 Gaokeyuan 3rd Road, East Lake High-Tech Zone, Wuhan City, Hubei Province, People's Republic of China.

Weigh 176g of sodium chloride and 88g of sodium citrate, dissolve in 800mL of deionized water, adjust the pH to 5.3±0.2 at room temperature, and complete to 1 L with deionized water. High-pressure steam sterilization, stored at 2-8°C, the solution shelf life is of 6 months. Discard if the reagent appears cloudy (turbid) or contaminated.

(2) $2 \times SSC$, pH 7.0 ± 0.2

Take 100mL of the above 20xSSC, dilute with 800mL deionized water, mix, adjust the pH to 7.0±0.2 at room temperature, complete to 1L with deionized water, stored at 2-8°C, the shelf life is of 6 months. Discard if the reagent appears cloudy (turbid) or contaminated.

(3) Ethanol Solution: 70% ethanol, 85% ethanol

Dilute 700ml, 850ml of ethanol with deionized water to 1L. The shelf life is of 6 months. Discard if the reagent appears cloudy (turbid) or contaminated.

(4) 0.3% NP-40/0.4xSSC solution, pH 7.0-7.5

Take 0.6mL NP-40 and 4mL 20×SSC, add 150mL deionized water, mix, adjust the pH to 7.0-7.5 at room temperature, with deionized water complete to a volume of 200mL. Stored at 2-8°C, the shelf life is of 6 months. Discard if the reagent appears cloudy (turbid) or contaminated.

(5) Fixation solution (methanol: glacial acetic acid = 3:1)

Prepare a ready to use fixation solution by mixing thoroughly 30ml of methanol and 10ml of glacial acetic acid.

(6) 0.075M KCl solution

Weigh 2.8g of potassium chloride, dissolve in 400mL of deionized water and complete to 500mL with deionized water. Stored at room temperature, the solution shelf life is of 6 months. Discard if the reagent appears cloudy (turbid) or contaminated.

(7) Diamidinyl phenylindole (DAPI) counterstain

Use commercially available anti-quenching DAPI counterstain.

2. Sample processing before hybridization:

Cells sample:

1. Sample processing before hybridization

- (1) Sample collection: take 1-3ml of heparin sodium anticoagulant bone marrow cells.
- (2) Cell harvesting: the uncultured marrow cells or the cultured marrow cell samples were aspirated to a 15mL centrifuged tube at the bottom of the tip, and centrifuged at 500g for 5min. The supernatant was carefully aspirated and discarded, leaving about 500μL of residual liquid to suspend the cells again.
- 3 Cell washing: add 5ml of 1xPBS buffer solution, blow and mix up the heavy suspension cell precipitation, centrifugate 500g for 5min, carefully suck and discard the supernatant, and leave about 500 μ L of residual solution to heavy suspension cell; repeat once.
- (4) Cell hypotonic: add 10ml of hypotonic solution to each tube (37°C warm bath in advance), and water bath at 37°C hypotonic for 20min.
- (5) Cell pre fixation: add 1ml (10% volume) of fixed solution to the cell suspension after hypotonic treatment, gently blow and mix, centrifugate 500g immediately for 5min, remove the supernatant, and leave about 500µL of residual solution for cell suspension.
- ⑥ Cell fixation: slowly add 10ml of the fixed solution to the cell suspension, leave it at room temperature for 10min to fix the cell, centrifugate 500g for 5min, and leave about 500μL of the residual solution to re suspend the cell; repeat once (or fix the cell several times until the cell is precipitated, washed and cleaned).
- 7 Preparation of cell suspension: after the last centrifugation of cell fixation, the supernatant is sucked off, and a proper amount of fixed solution is added to make cell suspension with appropriate concentration.
- (8) Preparation: take 3-10µL cell suspension drop to slide, aging at 56°C for 0.5h.
- (9) The slides were rinsed twice in 2xSSC solution at room temperature for 5min each time.
- (10) Dehydration: the cell drops were placed in 70% ethanol, 85% ethanol and 100% ethanol for 2 minutes respectively and then dried naturally. The following operations need to be carried out in the darkroom.

Cell sample:

- ① Take out the probe, leave it at room temperature for 5min, turn it upside down with force, mix it well, and then centrifuge it for a short time (no vortex instrument vibration). Take 10μ L of it and drop it into the cell drop hybridization area, immediately cover the cover glass of $22mm \times 22mm$. The probe should be evenly expanded under the cover glass without bubbles, and seal the edge with rubber glue (the edge must be completely sealed to prevent the dry piece from affecting the test results in the hybridization process).
- ② The cell drops were placed on the hybridizer and denatured at 88°C for 2min (the hybridizer should be preheated to 88°C) and hybridized at 45°C for 2 to 16 hours.

Wuhan HealthCare Biotechnology Co., Ltd.



Floor 1-4, Building #8, Optics Valley Precision Medicine Industry Base Phase I, #9 Gaokeyuan 3rd Road, East Lake High-Tech Zone, Wuhan City, Hubei Province, People's Republic of China.

Tissue samples:

- ① Take out the probe, let it stand at room temperature for 5min, turn it upside down with force, fully mix the probe, and then centrifuge briefly (vortex instrument oscillation is prohibited), take $10 \mu L$ was dropped on the hybridization area of cell drops and immediately covered with 22mm × For the 22mm cover glass, the probe shall be evenly expanded under the cover glass without bubbles, and the edge shall be sealed with rubber glue (the edge must be completely sealed to prevent the dry piece from affecting the test results during hybridization).
- 2 Put the tissue sections on the hybridizer, CO denature at 85 °C for 5min (the hybridizer should be preheated to 85 °C in advance), and hybridize at 42 °C for 2-16h.

3. Washing

The following operations need to be carried out in the darkroom.

- (1) Carefully remove the sealing glue around the cover glass with tweezers to avoid sticking or moving the cover glass, immerse the sample in 2xSSC for about 5S, take it out, gently push a corner of the cover glass to the edge of the slide with tweezers, and gently remove the cover glass with tweezers;
- (2) Place the sample at 2xSSC room temperature for 1 min;
- (3) Take out the sample and immerse it in 0.3%NP-40/0.4xSSC solution preheated at 68°C for 2min;
- 4) Take out the sample and immerse it in deionized water preheated at 37°C in advance for 1 min; dry it naturally in the dark environment.

5. Counterstaining


The following operations should be performed in a darkroom

10µl DAPI compound dye is dropped in the hybridization area of the glass slide and immediately covered. The suitable filter is selected for glass slide observation under the fluorescence microscope.

6. FISH results observation

Place the counterstained film under the fluorescence microscope, and first put it under the low-power objective lens ($10 \times$) Confirm the cell area under the microscope; Go to $40 \times$ Under the objective lens, find a position where the cells are evenly distributed; Then in the high-power objective ($100 \times$) The FISH results of nuclei were observed.

[Positive judgment value or reference interval]



[Limitations of test methods]

- ① The results of this kit will be affected by various factors of the sample itself, but also limited by hybridization temperature and time, operating environment and the limitations of current molecular biology technology, which may lead to wrong results.
- ② Users must understand the potential errors and accuracy limitations that may exist in the detection process.

[Precautions]

- 1. This product is only used for in vitro diagnosis.
- 2. Please read this manual carefully before testing. The testing personnel shall receive professional technical training, and the signal counting personnel must be able to observe and distinguish orange and green signals.
- 3. When testing clinical samples, when the hybridization signal counting is difficult and the sample is not enough to repeat the retest, or the cell volume is not enough for analysis, the test will not provide the test results.
- 4. Wear the mask with potential carcinogenicity during the operation of DAPI, and avoid direct contact with the mask with potential carcinogenicity.
- 5. All chemicals are potentially dangerous. Avoid direct contact. Used kits are clinical waste and should be properly disposed of..

[Basic information]

Name of registrant / manufacturer: Wuhan HealthCare Biotechnology Co., Ltd.

Address: Floor 1-4, Building #8, Optics Valley Precision Medicine Industry Base Phase I, #9 Gaokeyuan 3rd Road, East Lake High-Tech Zone, Wuhan City, Hubei Province, People's Republic of China.



Wuhan HealthCare Biotechnology Co., Ltd.

Floor 1-4, Building #8, Optics Valley Precision Medicine Industry Base Phase I, #9 Gaokeyuan 3rd Road, East Lake High-Tech Zone, Wuhan City, Hubei Province, People's Republic of China.

Contact: 027-87570662

Name of after-sales service unit: Wuhan HealthCare Biotechnology Co., Ltd.

Contact: 18140559890

Production address: Floor 1-4, Building #8, Optics Valley Precision Medicine Industry Base Phase I, #9 Gaokeyuan 3rd Road, East Lake High-

Tech Zone, Wuhan City, Hubei Province, People's Republic of China.

[medical device registration certificate No. / product technical requirement No.]

Medical device registration certificate No.: ehxb20190933
[approval date and modification date of the specification]

V1. 0 approval date: October 28, 2019 V1. 2 approval date: December 7, 2021